


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091523\
Data File : VV032110.D
Acq On : 15 Sep 2023 08:52
Operator : SY/MD
Sample : BFB213
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB213

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Title : VOC Analysis
Last Update : Sat Sep 16 02:09:37 2023

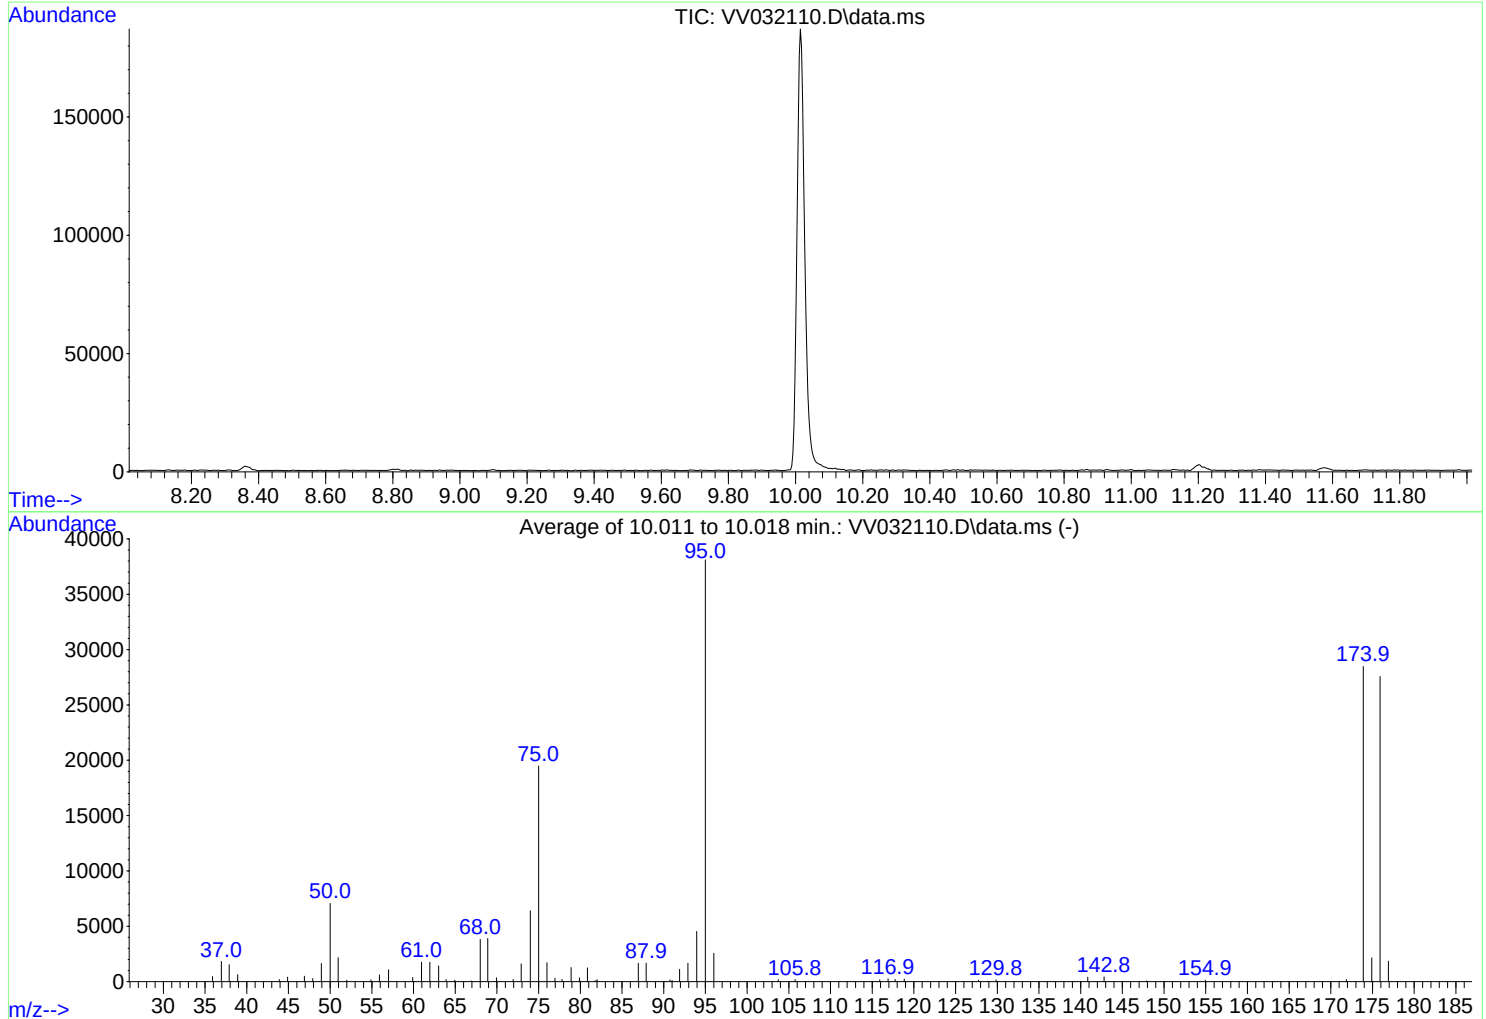

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2780

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	7074	PASS
75	95	30	80	51.1	19480	PASS
95	95	100	100	100.0	38107	PASS
96	95	5	9	6.7	2566	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.8	28485	PASS
175	174	5	9	7.6	2158	PASS
176	174	95	105	96.8	27568	PASS
177	176	5	10	6.7	1845	PASS

m/z	Abundance
39.10	132.0
39.90	185.0
43.90	532.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

m/z	Abundance
35.90	500.0
36.90	1807.0
37.90	1493.0
38.90	798.0
39.90	187.0
43.90	704.0
44.90	400.0
46.90	484.0
47.90	279.0
49.00	1609.0
50.00	7162.0
51.00	2183.0
52.00	126.0
54.90	206.0
55.90	619.0
57.00	1126.0
59.90	369.0
61.00	1775.0
61.90	1762.0
63.00	1423.0
63.90	167.0
65.00	121.0
66.90	124.0
68.00	3691.0
68.90	3830.0
70.00	344.0
72.00	192.0
72.90	1627.0
74.00	6207.0
75.00	19112.0
76.00	1661.0
77.00	354.0
77.80	195.0
78.90	1269.0
79.90	377.0
80.80	1206.0
81.80	256.0
86.90	1715.0
87.90	1622.0
90.80	153.0
91.90	1022.0
92.90	1660.0
93.90	4413.0
95.00	37104.0
96.00	2538.0
103.80	173.0
105.80	174.0
115.90	185.0
116.90	250.0
117.70	202.0
118.80	201.0
127.80	123.0
129.90	161.0
140.80	418.0
142.80	464.0
154.90	122.0
171.90	153.0
173.90	27176.0
174.90	2067.0
175.90	26304.0
176.90	1755.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

m/z	Abundance
35.90	483.0
37.00	1880.0
37.90	1571.0
38.90	792.0
39.90	185.0
43.90	742.0
44.90	430.0
46.90	496.0
47.90	299.0
48.90	1652.0
50.00	7291.0
50.90	2214.0
52.00	130.0
54.90	174.0
55.90	634.0
57.00	1093.0
59.90	382.0
61.00	1786.0
62.00	1819.0
63.00	1488.0
63.90	197.0
65.00	144.0
66.90	104.0
68.00	3977.0
68.90	4077.0
70.00	350.0
72.00	202.0
72.90	1654.0
74.00	6634.0
75.00	20160.0
76.00	1793.0
77.00	311.0
77.80	201.0
78.90	1318.0
79.90	358.0
80.80	1263.0
82.00	275.0
86.90	1670.0
87.90	1747.0
90.70	166.0
91.00	166.0
91.90	1155.0
92.90	1738.0
93.90	4687.0
95.00	39584.0
96.00	2656.0
103.80	180.0
105.70	193.0
115.90	174.0
116.90	265.0
117.70	218.0
118.80	245.0
127.70	122.0
129.90	171.0
140.90	421.0
142.80	451.0
147.90	113.0
155.00	138.0
171.80	201.0
173.90	29480.0
174.90	2216.0
175.90	28552.0
176.90	1879.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213

m/z	Abundance
35.90	406.0
36.90	1784.0
37.90	1518.0
38.90	699.0
40.00	183.0
43.90	730.0
44.90	380.0
46.90	482.0
47.90	257.0
48.90	1650.0
50.00	6768.0
50.90	2100.0
52.00	117.0
54.90	146.0
55.90	566.0
57.00	979.0
59.90	387.0
60.90	1701.0
62.00	1662.0
63.00	1341.0
63.90	195.0
64.90	147.0
68.00	3785.0
68.90	3810.0
69.90	339.0
71.90	200.0
72.90	1546.0
74.00	6385.0
75.00	19168.0
76.00	1678.0
76.80	270.0
77.80	195.0
78.90	1238.0
79.90	326.0
80.90	1248.0
82.00	302.0
87.00	1596.0
87.90	1654.0
90.70	156.0
91.00	155.0
91.90	1185.0
92.90	1582.0
94.00	4507.0
95.00	37632.0
96.00	2503.0
103.70	191.0
105.70	194.0
115.90	143.0
116.90	256.0
117.80	191.0
118.90	251.0
127.70	135.0
128.80	111.0
129.80	141.0
140.80	387.0
142.80	398.0
147.90	112.0
155.00	138.0
171.80	216.0
173.90	28800.0
174.90	2192.0
175.90	27848.0
176.90	1901.0

Instrument :
MSVOA_V
ClientSampleId :
BFB213