
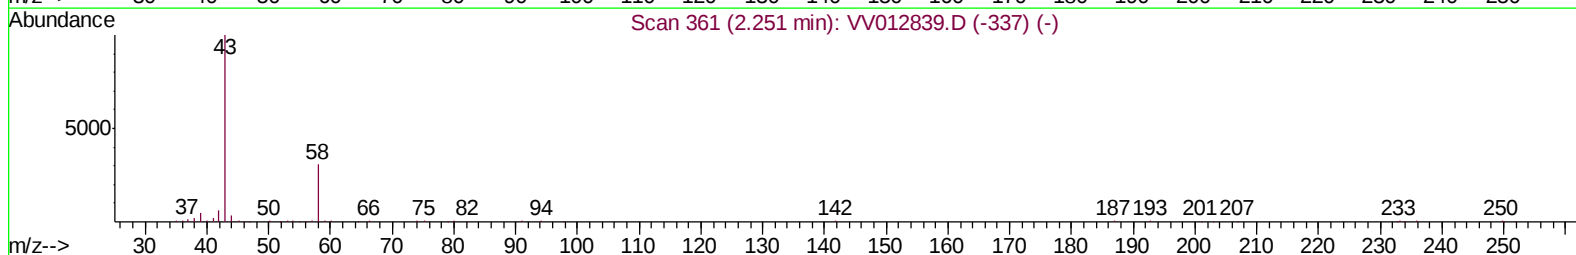
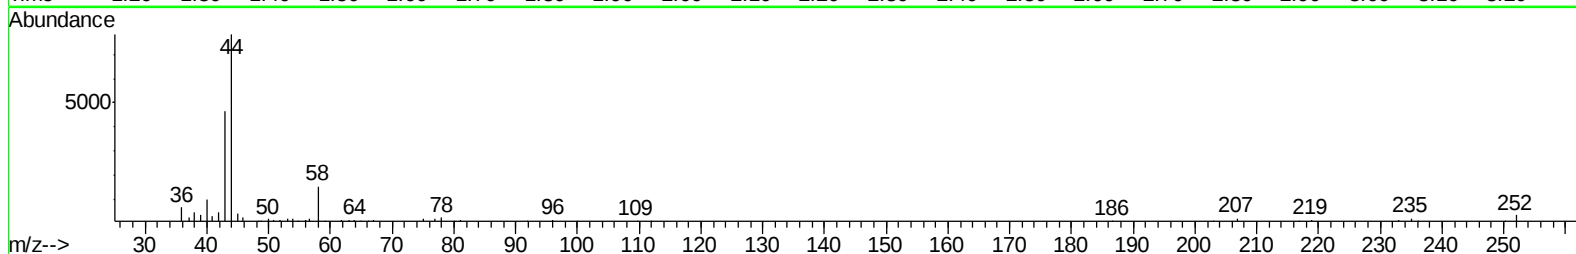


Data File : VV012858.D
Acq On : 17 Sep 2019 01:20
Operator : SY/MD
Sample : K4834-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Quant Time: Sep 17 07:28:29 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Sep 17 07:22:21 2019
Response via : Initial Calibration

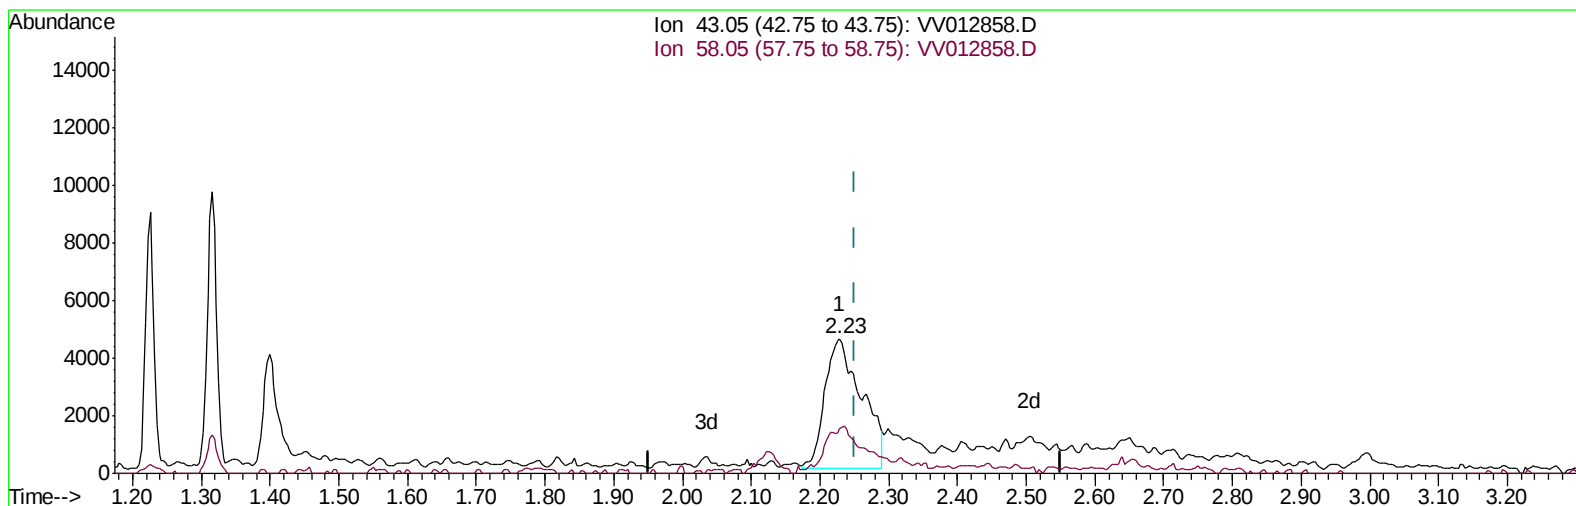

TIC: VV012858.D

(13) Acetone (T)

2.229min (-0.023) 5.84ug/L m

response 16678

Ion	Exp%	Act%
43.05	100	100
58.05	28.30	33.81
0.00	0.00	0.00
0.00	0.00	0.00