


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091619\
 Data File : VV012862.D
 Acq On : 17 Sep 2019 03:33
 Operator : SY/MD
 Sample : VSTDCCC005EC
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Quant Time: Sep 17 09:16:48 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091619WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Sep 17 07:22:21 2019
 Response via : Initial Calibration

Instrument :
 MSVOA_V
 LabSampleId :
 VSTD00559

Manual Integrations
 APPROVED

MMDadoda
 9/17/2019 10:47:28 AM

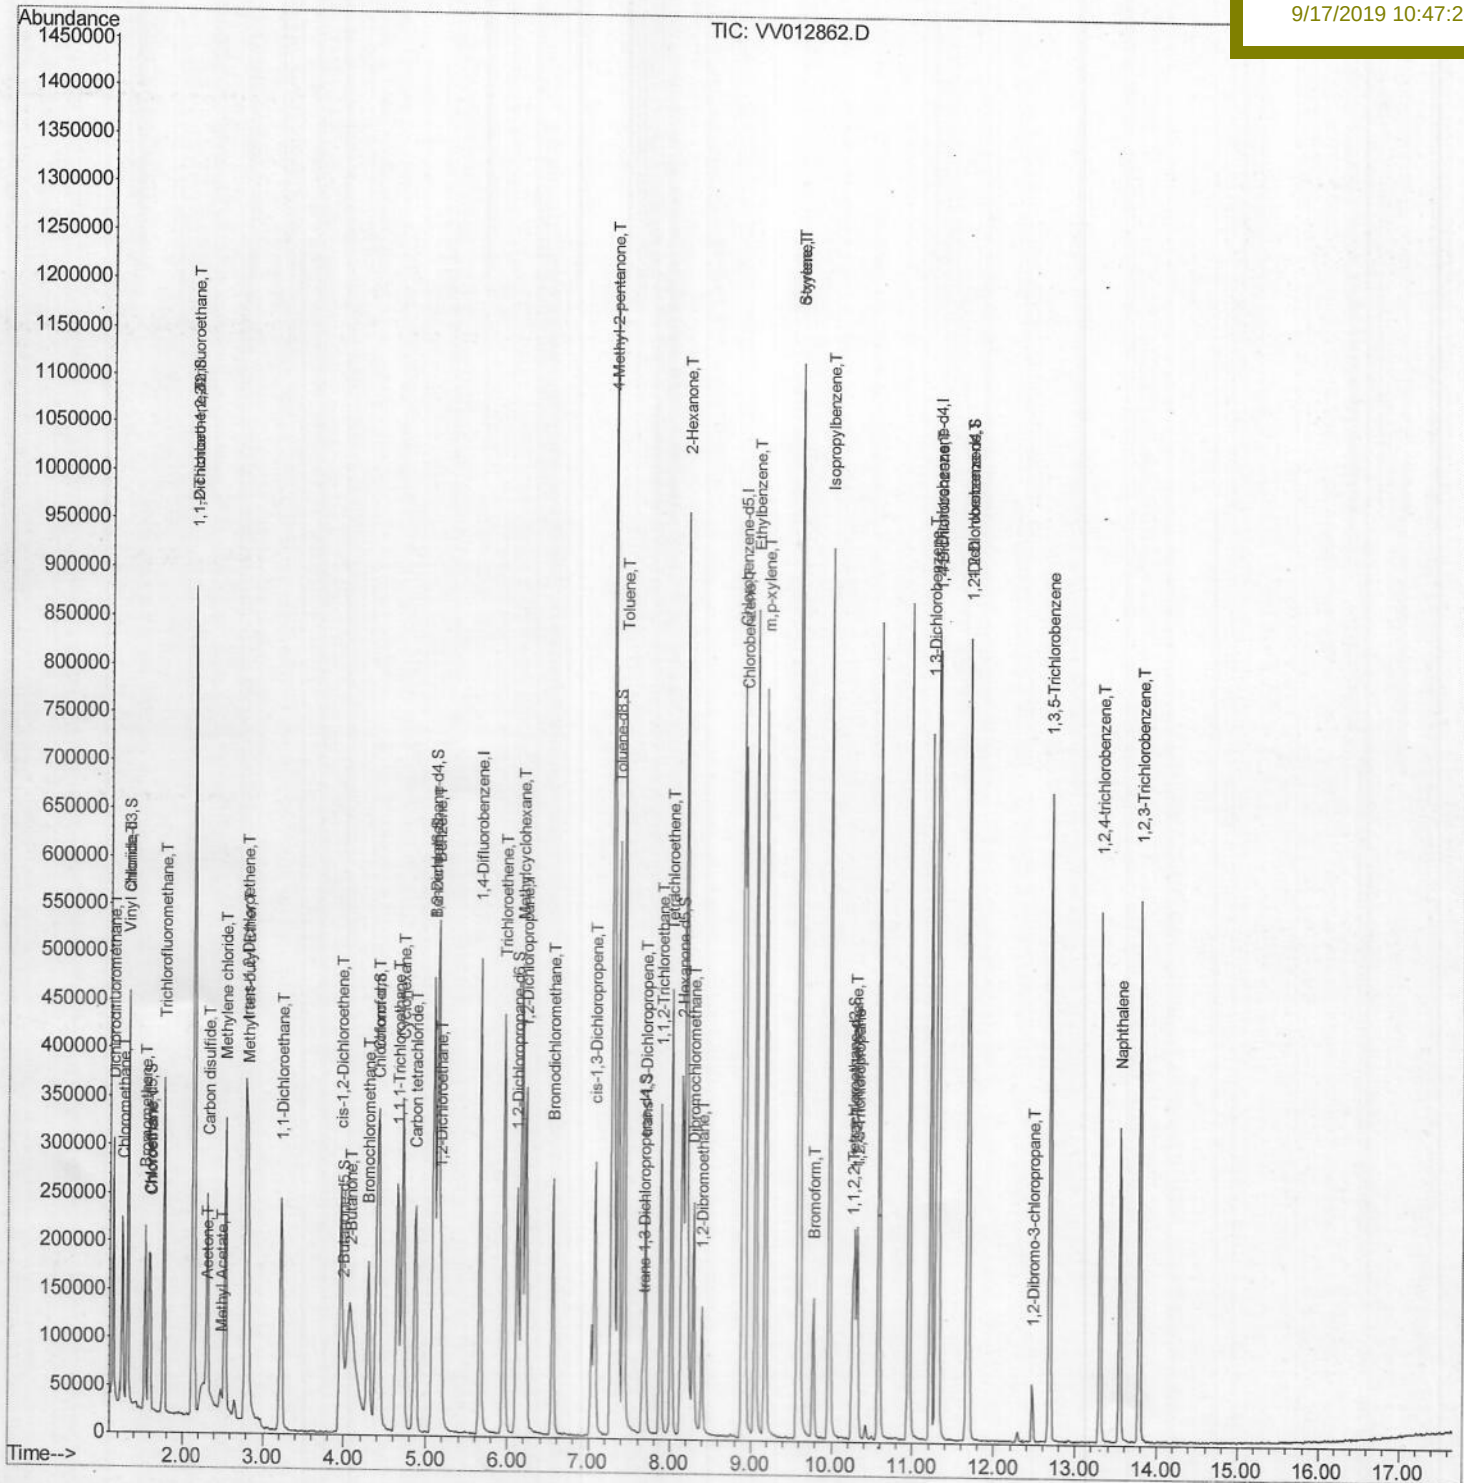

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091619\

Data File : VV012862.D

Acq On : 17 Sep 2019 03:33

Operator : SY/MD

Sample : VSTDCCC005EC

Misc : 25.0mL/MSVOA_V/WATER

ALS Vial : 42 Sample Multiplier: 1

Quant Time: Sep 17 07:29:09 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091619WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Tue Sep 17 07:22:21 2019




Response via : Initial Calibration

Instrument :

MSVOA_V

LabSampleId :

VSTD00559

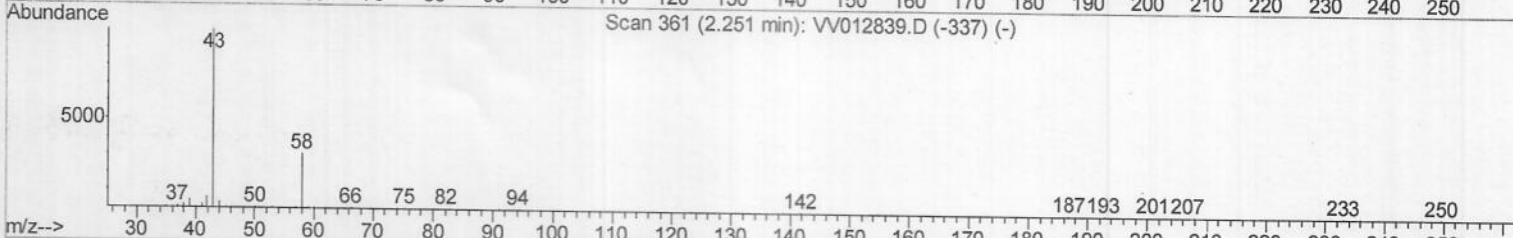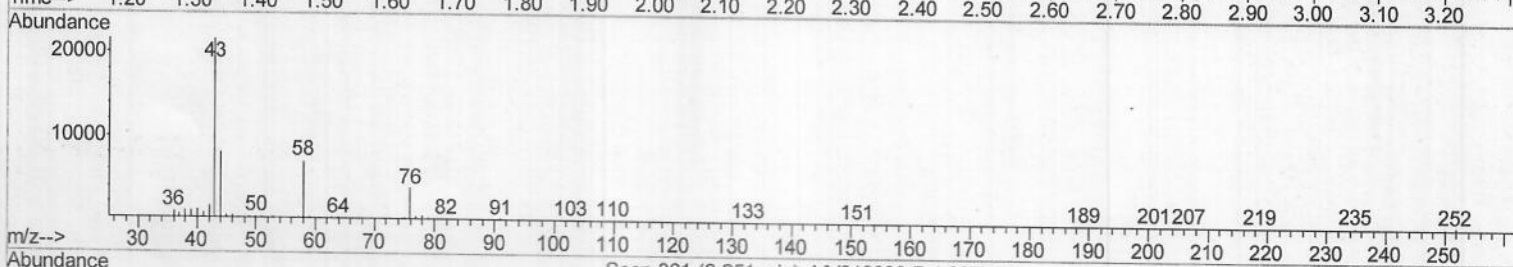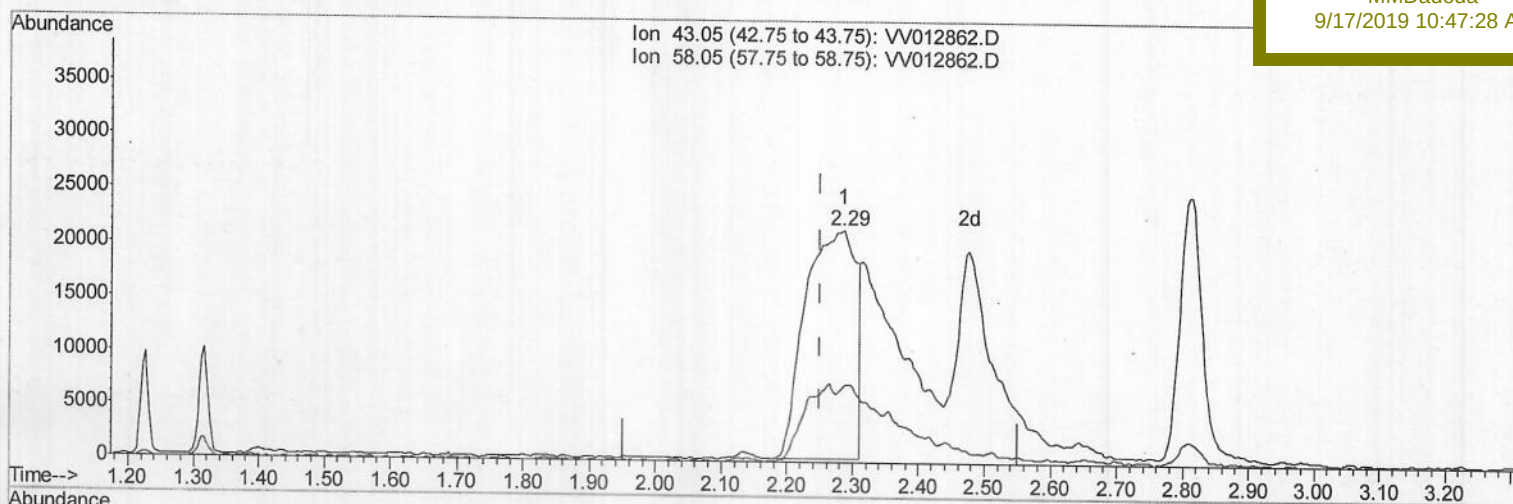Manual Integrations
APPROVEDMMDadoda
9/17/2019 10:47:28 AM

TIC: VV012862.D

(13) Acetone (T)

2.286min (+0.035) 36.63ug/L

response 112484

Ion	Exp%	Act%
43.05	100	100
58.05	28.30	9.32
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091619\
Data File : VV012862.D
Acq On : 17 Sep 2019 03:33
Operator : SY/MD
Sample : VSTDCCC005EC
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Quant Time: Sep 17 07:29:09 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Sep 17 07:22:21 2019
Response via : Initial Calibration

Instrument :
MSVOA_V
LabSampleId :
VSTD00559

Manual Integrations
APPROVED

MMDadoda
9/17/2019 10:47:28 AM

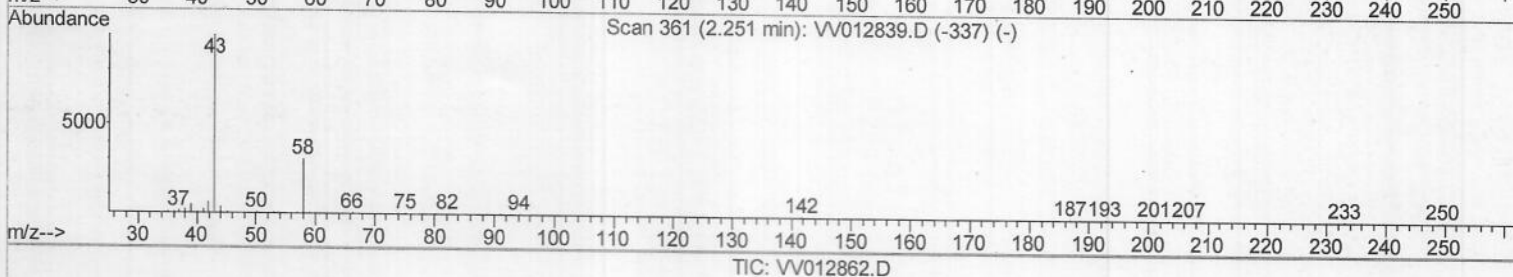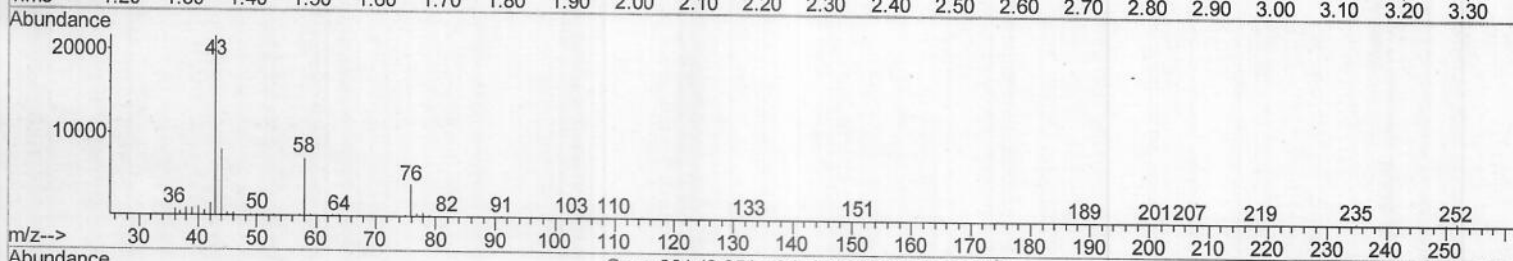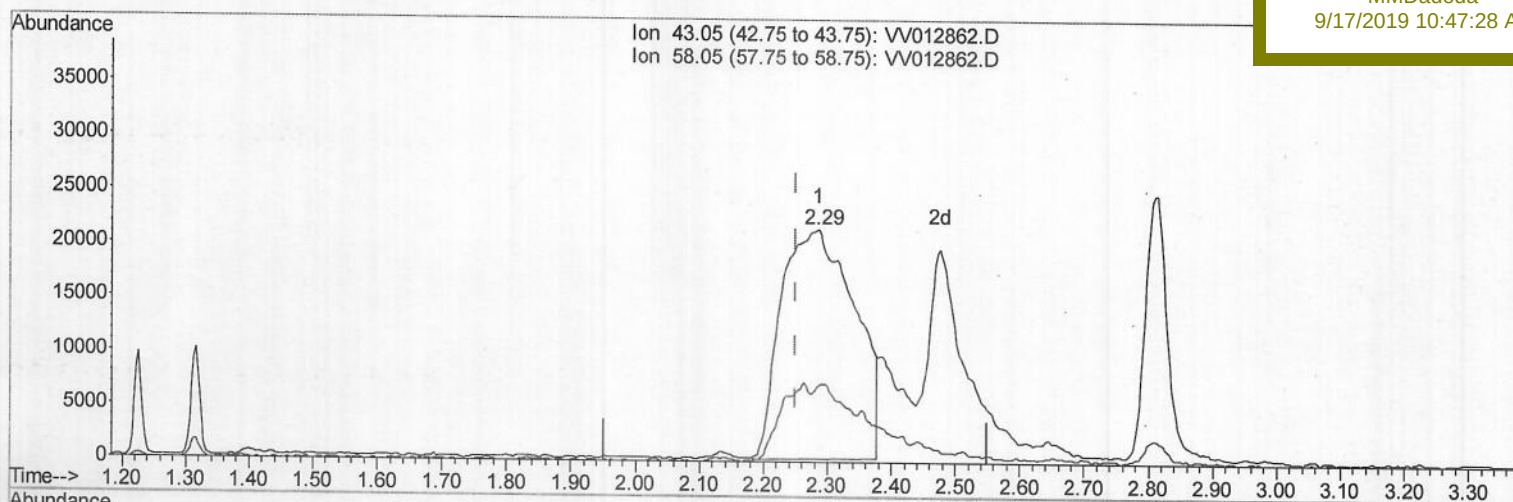

(13) Acetone (T)

2.286min (+0.035) 55.40ug/L m

S.M.D 09/17/19

response 170149

Ion	Exp%	Act%
43.05	100	100
58.05	28.30	6.16
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091619\
Data File : VV012862.D
Acq On : 17 Sep 2019 03:33
Operator : SY/MD
Sample : VSTDCCC005EC
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Quant Time: Sep 17 07:29:09 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Sep 17 07:22:21 2019
Response via : Initial Calibration

Instrument :
MSVOA_V
LabSampleId :
VSTD00559

Manual Integrations
APPROVED

MMDadoda
9/17/2019 10:47:28 AM

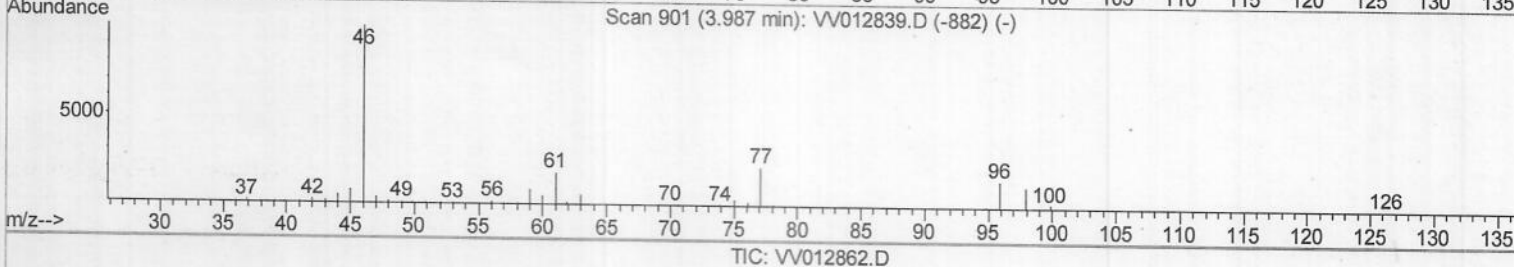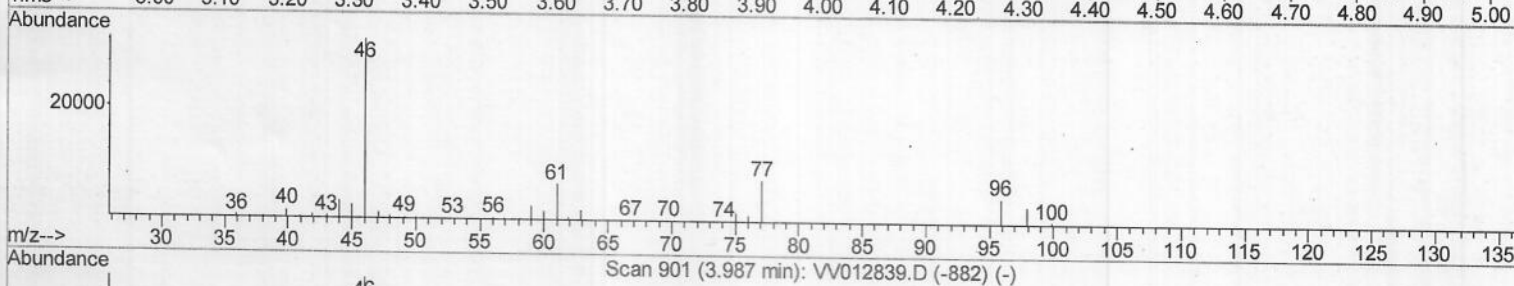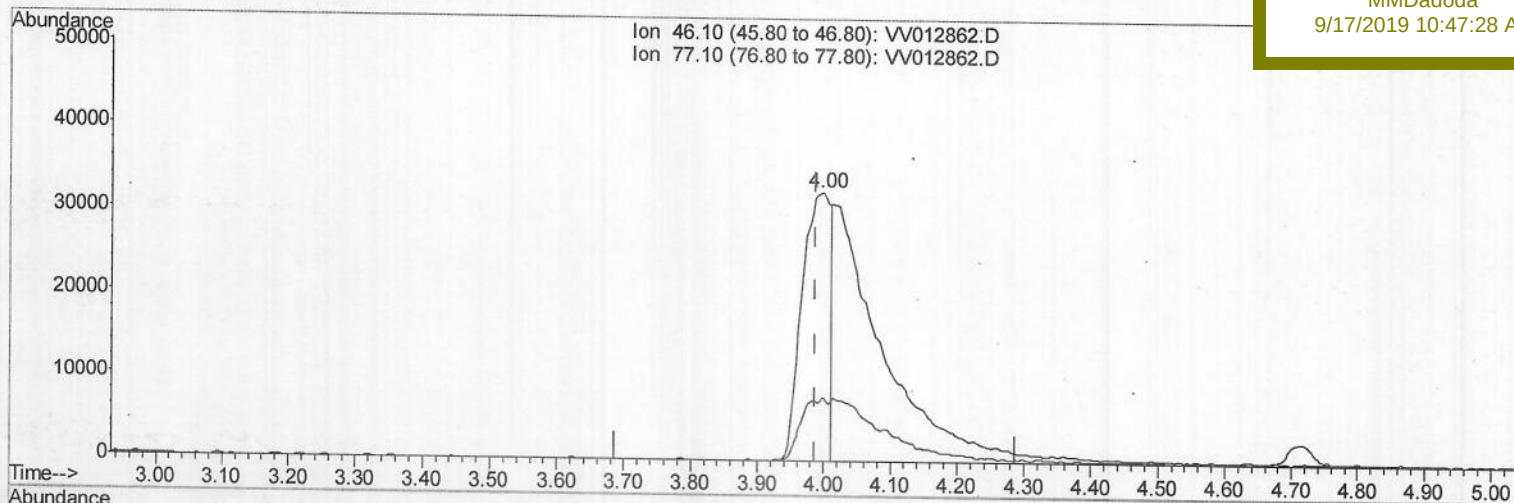

(20) 2-Butanone-d5 (S)

3.997min (+0.010) 23.53ug/L

response 93253

Ion	Exp%	Act%
46.10	100	100
77.10	23.30	14.29#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091619\

Data File : VV012862.D

Acq On : 17 Sep 2019 03:33

Operator : SY/MD

Sample : VSTDCCC005EC

Misc : 25.0mL/MSVOA_V/WATER

ALS Vial : 42 Sample Multiplier: 1

Quant Time: Sep 17 07:29:09 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091619WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Tue Sep 17 07:22:21 2019

Response via : Initial Calibration

Instrument :

MSVOA_V

LabSampleId :




VSTD00559

Manual Integrations

APPROVED

MMDadoda

9/17/2019 10:47:28 AM

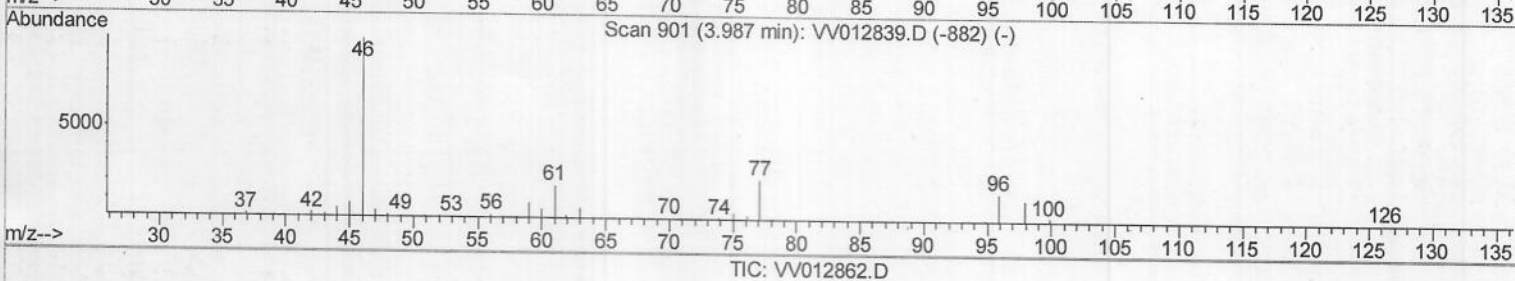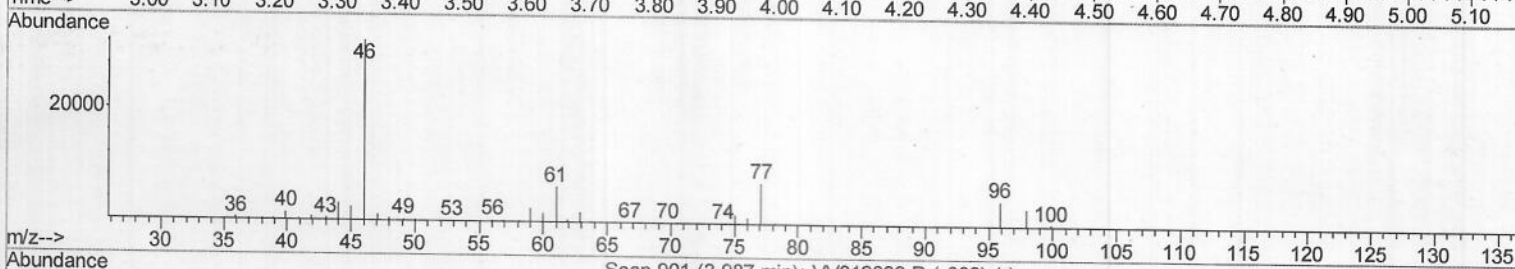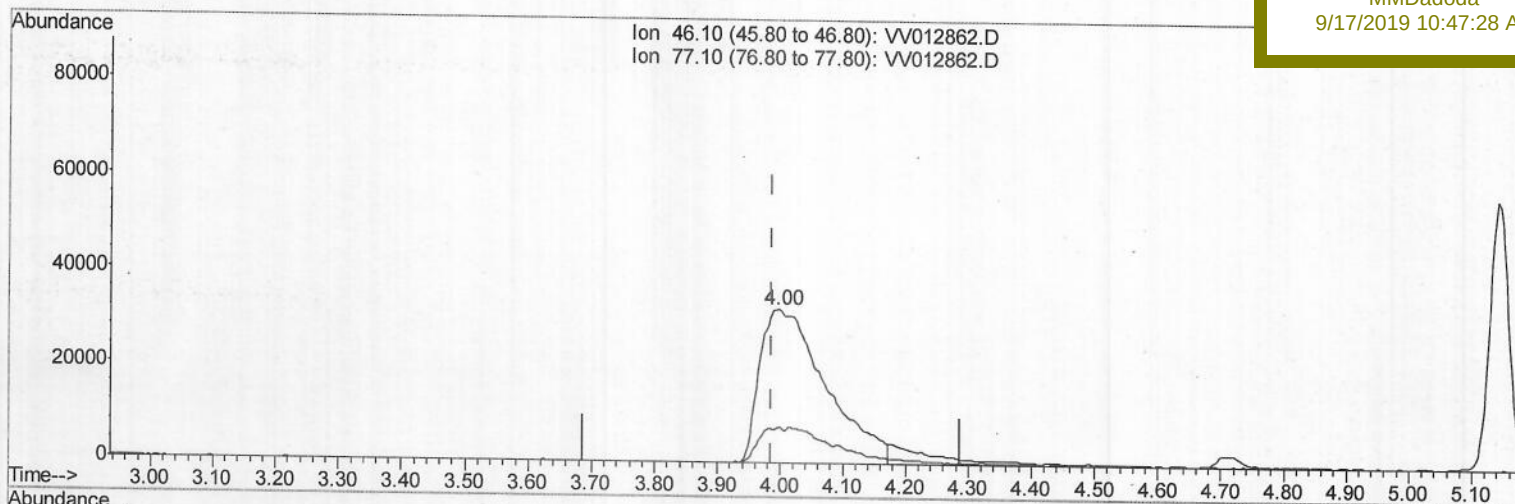

(20) 2-Butanone-d5 (S)

3.997min (+0.010) 59.71ug/L m

response 236641

Ion	Exp%	Act%
46.10	100	100
77.10	23.30	5.63#
0.00	0.00	0.00
0.00	0.00	0.00

M.D 09/18/19

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091619\
 Data File : VV012862.D
 Acq On : 17 Sep 2019 03:33
 Operator : SY/MD
 Sample : VSTDCCC005EC
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 LabSampleId :
 VSTD00559

Manual Integrations
 APPROVED

MMDadoda
 9/17/2019 10:47:28 AM

Quant Time: Sep 17 09:16:48 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091619WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Sep 17 07:22:21 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.66	114	414024	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	415170	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	203472	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	123972	4.32	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.40%
7) Chloroethane-d5	1.58	69	96266	4.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.60%
11) 1,1-Dichloroethene-d2	2.13	63	207201	4.36	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	87.20%
20) 2-Butanone-d5	4.00	46	236641m	59.71	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.42%
24) Chloroform-d	4.40	84	208982	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.80%
26) 1,2-Dichloroethane-d4	5.08	65	98735	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.20%
32) Benzene-d6	5.09	84	404211	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.20%
36) 1,2-Dichloropropane-d6	6.12	67	124340	4.50	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.00%
41) Toluene-d8	7.36	98	385424	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.60%
43) trans-1,3-Dichloropropene-	7.66	79	39978	4.48	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.60%
46) 2-Hexanone-d5	8.14	63	134398	53.76	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.52%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	77396	5.10	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	130744	4.63	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.60%

> M.D 09/18/19

Target Compounds

					Qvalue
2) Dichlorodifluoromethane	1.14	85	148457	4.749 ug/L	100
3) Chloromethane	1.25	50	140621	4.631 ug/L	95
5) Vinyl chloride	1.32	62	158035	4.641 ug/L	99
6) Bromomethane	1.53	94	81436	4.652 ug/L	98
8) Chloroethane	1.60	64	85010	4.627 ug/L	97
9) Trichlorofluoromethane	1.77	101	196857	4.728 ug/L	98
10) 1,1,2-Trichloro-1,2,2-trif	2.14	101	113874	4.625 ug/L	97
12) 1,1-Dichloroethene	2.14	96	107622	4.759 ug/L	97
13) Acetone	2.29	43	170149m	55.403 ug/L	97
14) Carbon disulfide	2.31	76	221002	4.538 ug/L	99
15) Methyl Acetate	2.48	43	64859	7.306 ug/L	90
16) Methylene chloride	2.53	84	124435	4.625 ug/L	99
17) Methyl tert-butyl Ether	2.81	73	312362	5.286 ug/L	99
18) trans-1,2-Dichloroethene	2.78	96	115298	4.670 ug/L	98
19) 1,1-Dichloroethane	3.22	63	249566	4.905 ug/L	98
21) 2-Butanone	4.07	43	394051	70.335 ug/L	91
22) cis-1,2-Dichloroethene	3.96	96	133065	4.883 ug/L	97

> M.D 09/18/19

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091619\
 Data File : VV012862.D
 Acq On : 17 Sep 2019 03:33
 Operator : SY/MD
 Sample : VSTDCCC005EC
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 LabSampleId :
 VSTD00559

Quant Time: Sep 17 09:16:48 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091619WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Sep 17 07:22:21 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 9/17/2019 10:47:28 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
23) Bromochloromethane	4.29	128	61327	5.183	ug/L	99
25) Chloroform	4.42	83	265950	4.681	ug/L	99
27) 1,2-Dichloroethane	5.18	62	154777	5.261	ug/L	99
29) 1,1,1-Trichloroethane	4.65	97	202210	4.743	ug/L	99
30) Cyclohexane	4.72	56	172339	4.774	ug/L	97
31) Carbon tetrachloride	4.87	117	171550	4.745	ug/L	100
33) Benzene	5.14	78	519391	4.951	ug/L	100
34) Trichloroethene	5.96	95	146486	4.893	ug/L	98
35) Methylcyclohexane	6.17	83	175602	4.774	ug/L	99
37) 1,2-Dichloropropane	6.22	63	140970	4.993	ug/L	99
38) Bromodichloromethane	6.55	83	177689	4.865	ug/L	99
39) cis-1,3-Dichloropropene	7.07	75	169343	4.840	ug/L	99
40) 4-Methyl-2-pentanone	7.28	43	967006	61.954	ug/L	98
42) Toluene	7.43	91	559049	5.212	ug/L	99
44) trans-1,3-Dichloropropene	7.69	75	135983	4.887	ug/L	100
45) 1,1,2-Trichloroethane	7.88	97	102232	5.088	ug/L	99
47) Tetrachloroethene	8.02	164	105736	4.822	ug/L	98
48) 2-Hexanone	8.19	43	733857	61.677	ug/L	99
49) Dibromochloromethane	8.29	129	117866	5.129	ug/L	97
50) 1,2-Dibromoethane	8.40	107	86403	5.165	ug/L	98
51) Chlorobenzene	8.92	112	363996	4.912	ug/L	97
52) Ethylbenzene	9.05	91	581548	5.083	ug/L	100
53) m,p-xylene	9.18	106	221463	5.211	ug/L	98
54) o-xylene	9.59	106	216415	5.237	ug/L	98
55) Styrene	9.60	104	384885	5.490	ug/L	99
56) Isopropylbenzene	9.97	105	577125	5.208	ug/L	100
58) 1,1,2,2-Tetrachloroethane	10.28	83	99598	5.315	ug/L	98
59) 1,2,3-Trichloropropane	10.32	75	88956	5.319	ug/L	99
61) Bromoform	9.77	173	63860	5.037	ug/L	98
62) 1,3-Dichlorobenzene	11.22	146	297157	5.106	ug/L	99
63) 1,4-Dichlorobenzene	11.31	146	296283	4.921	ug/L	98
65) 1,2-Dichlorobenzene	11.69	146	284357	5.044	ug/L	100
66) 1,2-Dibromo-3-chloropropan	12.47	75	13783	5.100	ug/L	97
67) 1,3,5-Trichlorobenzene	12.69	180	211994	4.733	ug/L	99
68) 1,2,4-trichlorobenzene	13.31	180	167716	4.994	ug/L	99
69) Naphthalene	13.55	128	256910	5.350	ug/L	100
70) 1,2,3-Trichlorobenzene	13.79	180	172627	5.294	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed