

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091619\
 Data File : VV012849.D
 Acq On : 16 Sep 2019 21:22
 Operator : SY/MD
 Sample : K4834-03
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0MD8

Quant Time: Sep 17 08:11:20 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091619WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Sep 17 07:22:21 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	393181	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	387704	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	142343	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	123573	4.54	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.80%
7) Chloroethane-d5	1.58	69	102243	4.79	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.80%
11) 1,1-Dichloroethene-d2	2.13	63	161004	3.57	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.40%
20) 2-Butanone-d5	3.97	46	213427	56.70	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.40%
24) Chloroform-d	4.40	84	202246	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.60%
26) 1,2-Dichloroethane-d4	5.08	65	103159	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.80%
32) Benzene-d6	5.09	84	413193	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
36) 1,2-Dichloropropane-d6	6.12	67	127891	4.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.20%
41) Toluene-d8	7.36	98	319987	4.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.20%
43) trans-1,3-Dichloropropene-	7.67	79	40085	4.81	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.20%
46) 2-Hexanone-d5	8.14	63	111185	47.62	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.24%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	74397	5.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	110342	5.59	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.80%


Target Compounds					Ovalue
13) Acetone	2.22	43	14224	4.877 ug/L	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091619\
Data File : VV012849.D
Acq On : 16 Sep 2019 21:22
Operator : SY/MD
Sample : K4834-03
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MD8

Quant Time: Sep 17 08:11:20 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Sep 17 07:22:21 2019
Response via : Initial Calibration

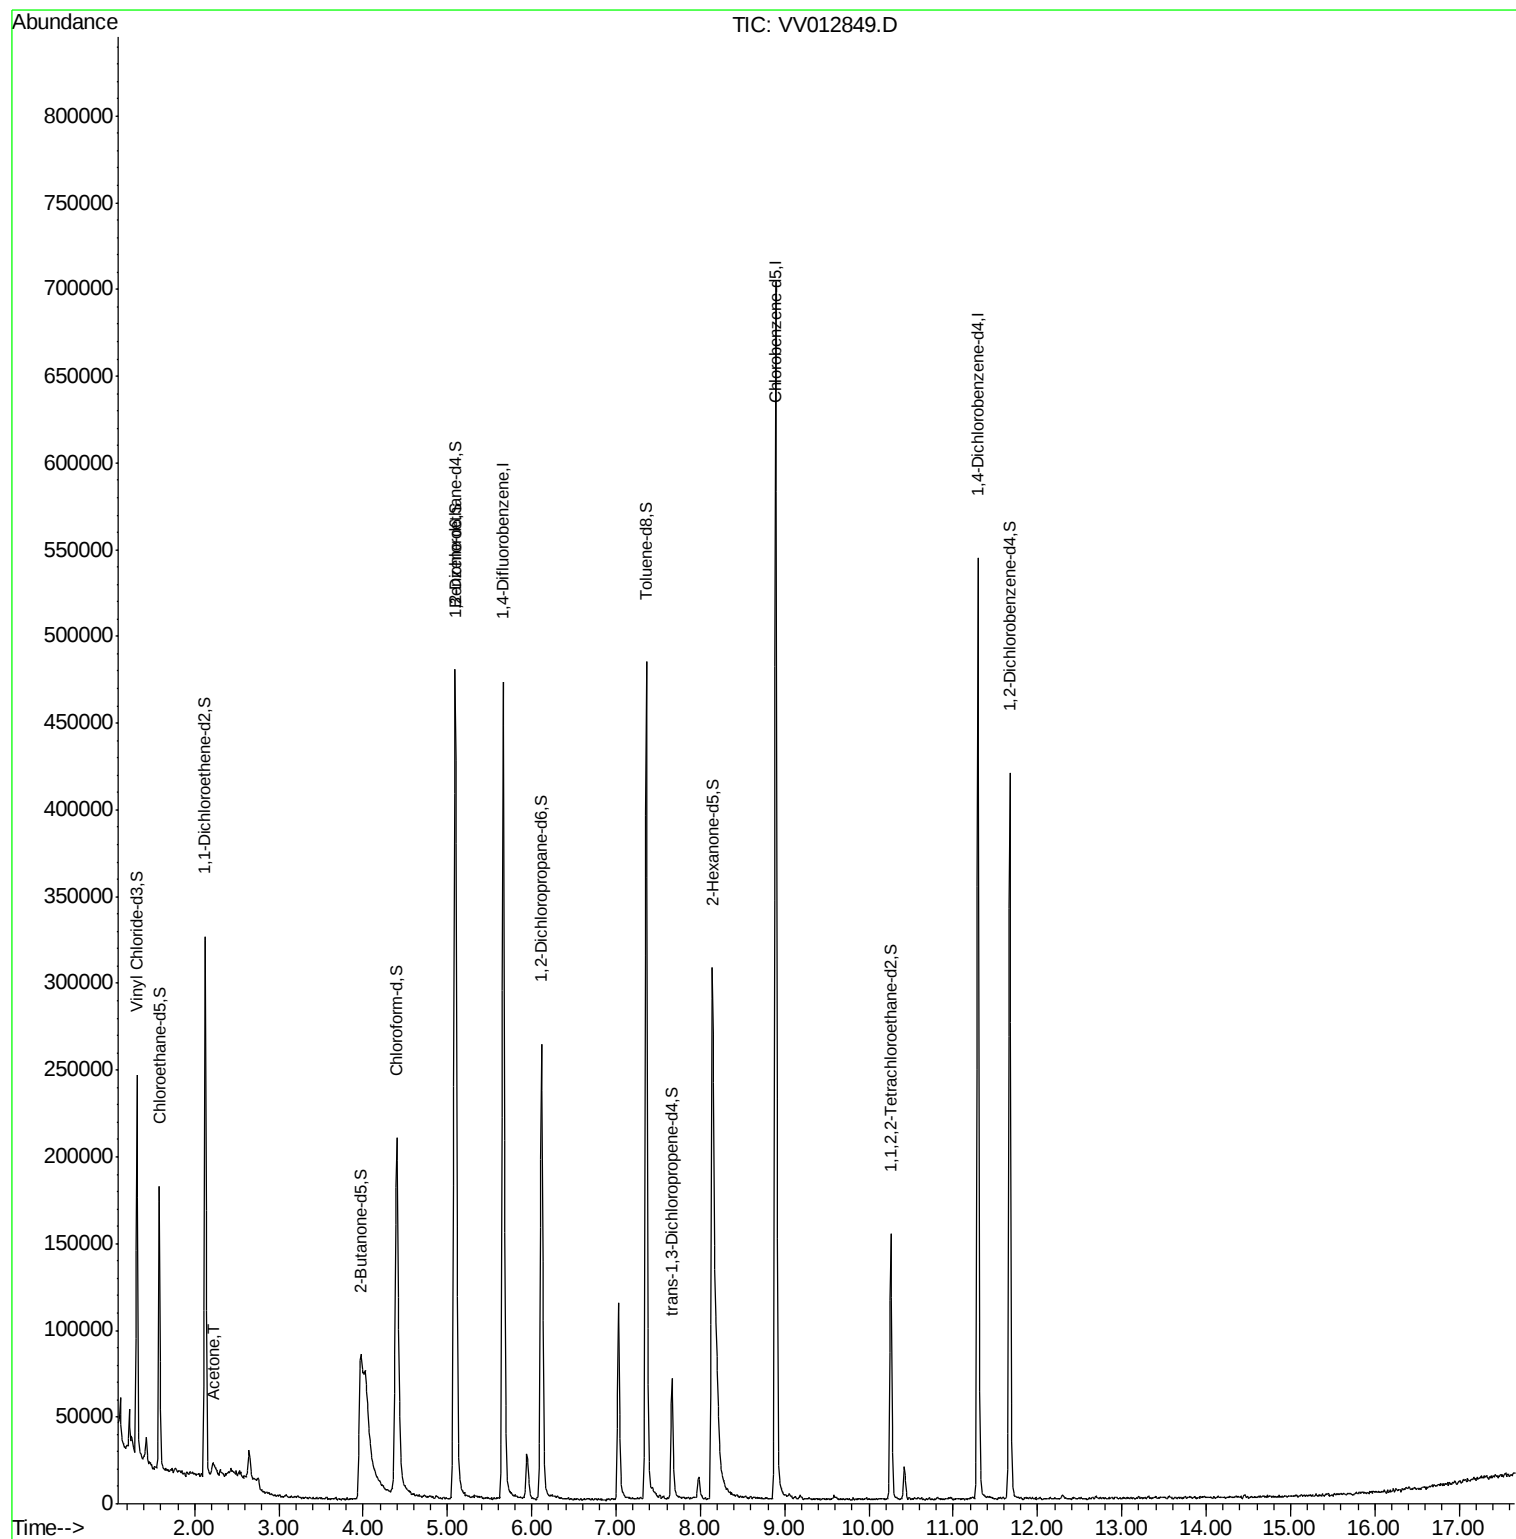

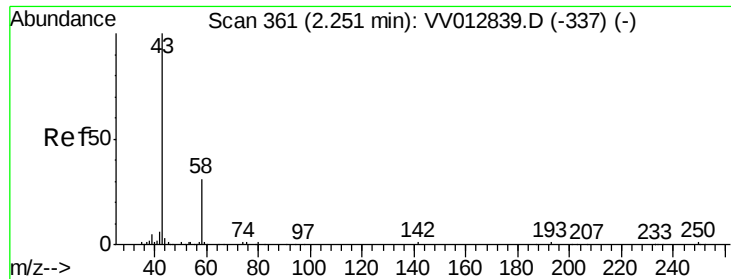

#13

Acetone

Concen: 4.877 ug/L

RT: 2.22 min Scan# 351

Delta R.T. -0.03 min

Lab File: VV012849.D

Acq: 16 Sep 2019 21:22

Instrument :

MSVOA_V

ClientSampleId :

C0MD8

Tot Ion: 43 Resp: 14224

Ion Ratio Lower Upper

43 100

58 15.8 0.0 56.6

