


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV091619\
 Data File : VV012824.D
 Acq On : 16 Sep 2019 08:35
 Operator : SY/MD
 Sample : BFB38
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB38

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091619WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Sep 17 07:22:21 2019

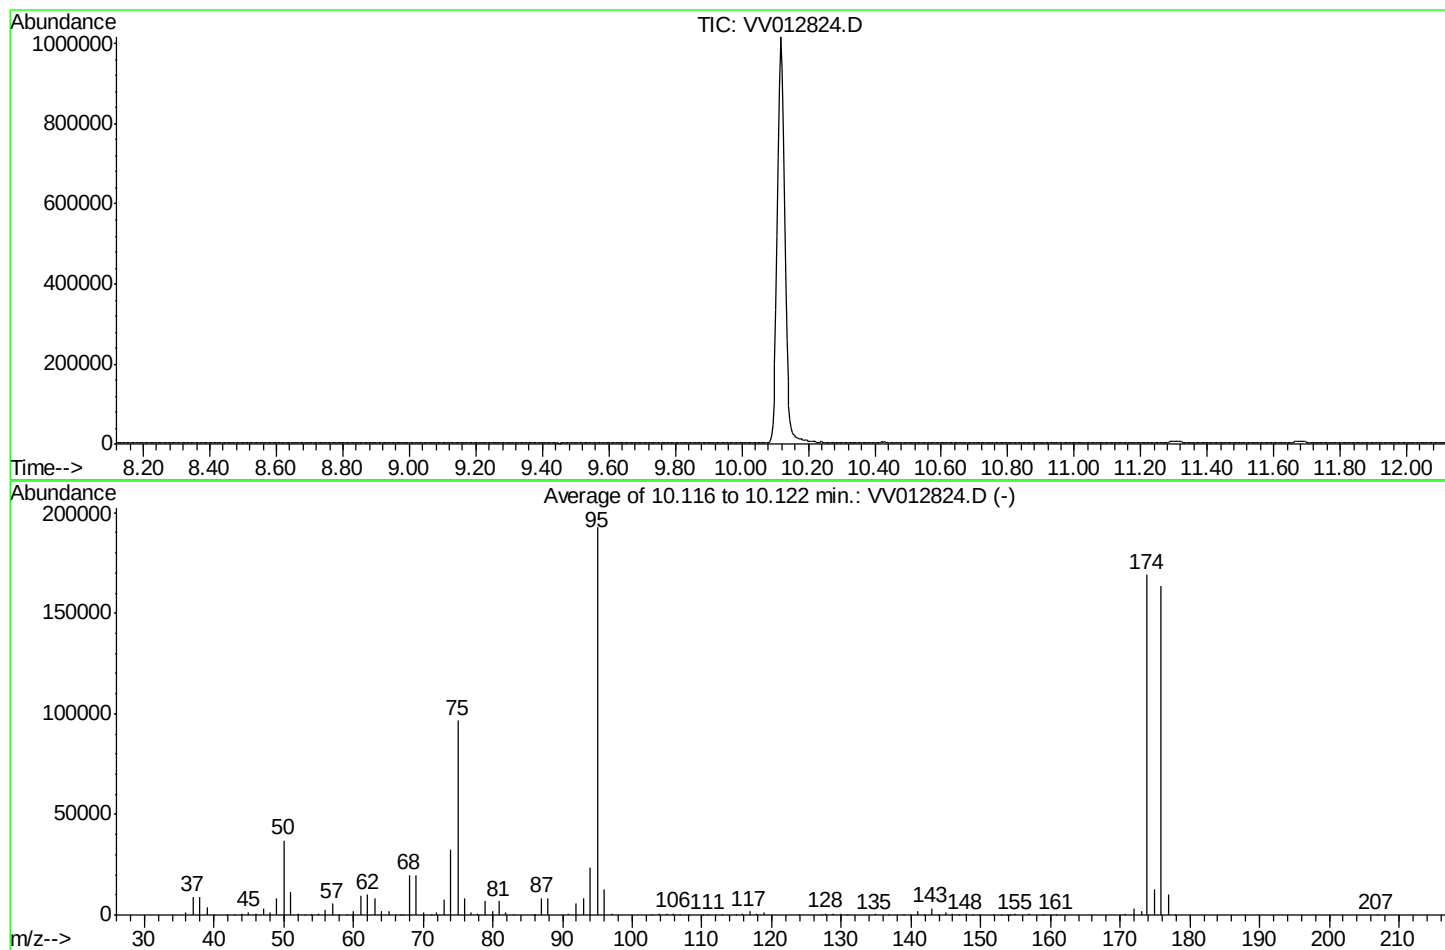

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	37024	PASS
75	95	30	80	50.1	96589	PASS
95	95	100	100	100.0	192704	PASS
96	95	5	9	6.6	12643	PASS
173	174	0.00	2	1.2	2054	PASS
174	95	50	120	87.7	168960	PASS
175	174	5	9	7.7	13032	PASS
176	174	95	101	96.8	163477	PASS
177	176	5	9	6.4	10471	PASS

m/z	Abundance
36.00	1917.0
37.00	9190.0
38.00	9250.0
39.00	4224.0
40.00	1246.0
41.80	104.0
43.00	171.0
44.00	1810.0
45.00	1629.0
46.00	423.0
47.00	3050.0
48.00	1670.0
49.00	8847.0
50.00	38872.0
51.00	11719.0
52.10	612.0
52.90	341.0
53.90	164.0
55.00	483.0
56.00	2879.0
57.00	5615.0
58.00	266.0
58.90	124.0
60.00	2133.0
61.00	9845.0
62.00	10721.0
63.00	8484.0
64.00	1843.0
65.10	2144.0
66.10	252.0
66.90	482.0
68.00	20200.0
69.00	19976.0
70.00	1470.0
72.00	998.0
73.00	8259.0
74.00	33128.0
75.00	99864.0
76.00	8108.0
76.90	1119.0
77.90	836.0
78.90	7214.0
79.90	1919.0
80.90	7088.0
81.90	1678.0
82.90	114.0
85.80	337.0
87.00	8454.0
87.90	8645.0
90.90	735.0
92.00	5769.0
93.00	8603.0
94.00	23864.0
95.00	197376.0
96.00	13105.0
97.00	376.0
102.70	155.0
103.90	912.0
104.90	402.0
105.90	870.0
106.80	255.0
108.00	170.0
110.10	156.0
110.90	267.0
112.00	157.0
112.90	237.0
114.80	265.0
115.80	584.0
116.90	1765.0
117.90	752.0
118.90	1473.0
123.80	135.0
127.10	129.0
127.80	753.0
128.90	417.0
129.90	609.0
130.80	312.0
134.90	460.0
136.80	295.0
138.90	102.0
139.80	168.0
140.90	1888.0
141.80	220.0
142.90	3445.0
143.80	272.0
144.90	1186.0
145.90	355.0
146.70	141.0
147.80	516.0
148.90	189.0
150.00	254.0
151.80	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

152.80	124.0
153.80	174.0
155.00	524.0
156.90	401.0
159.00	255.0
160.80	311.0
170.80	502.0
171.90	2822.0
173.00	2214.0
173.90	167680.0
174.90	13280.0
175.90	161536.0
176.90	10782.0
177.90	257.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

m/z	Abundance
36.00	1783.0
37.00	9324.0
38.00	9146.0
39.00	4082.0
40.00	1282.0
41.90	114.0
42.90	180.0
44.00	1799.0
45.00	1618.0
46.00	443.0
47.10	3031.0
47.90	1659.0
49.00	8602.0
50.00	38208.0
51.00	11858.0
52.00	559.0
52.90	349.0
54.00	174.0
55.00	513.0
56.00	2933.0
57.00	5670.0
58.00	270.0
59.00	116.0
60.00	2054.0
61.00	10104.0
62.00	10366.0
63.00	8523.0
64.00	1761.0
65.10	2161.0
66.10	257.0
66.80	452.0
68.00	20432.0
69.00	20112.0
70.00	1585.0
71.90	1060.0
73.00	7823.0
74.00	33384.0
75.00	99880.0
76.00	8337.0
76.90	1068.0
77.80	761.0
78.90	7140.0
79.90	1899.0
80.90	6904.0
81.90	1602.0
83.00	138.0
86.00	346.0
87.00	8616.0
87.90	8521.0
90.90	752.0
92.00	5690.0
93.00	8751.0
94.00	24352.0
95.00	199168.0
96.00	12912.0
97.00	362.0
102.70	155.0
103.90	918.0
104.90	376.0
105.90	944.0
106.70	237.0
108.00	167.0
110.10	196.0
110.80	289.0
112.00	182.0
112.90	228.0
114.90	291.0
115.80	578.0
116.90	1705.0
117.90	739.0
118.90	1513.0
123.80	191.0
127.10	126.0
127.80	746.0
128.90	419.0
129.90	697.0
130.80	343.0
134.90	453.0
136.80	291.0
139.90	205.0
140.90	1854.0
141.90	234.0
142.90	3430.0
143.80	264.0
144.90	1183.0
145.90	452.0
146.80	154.0
147.90	503.0
148.80	166.0
149.80	284.0
151.80	135.0
152.80	178.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

153.80	167.0
154.90	628.0
156.90	472.0
159.00	335.0
160.80	305.0
170.70	521.0
171.90	2981.0
173.00	2087.0
173.90	174272.0
174.90	13518.0
175.90	169216.0
177.00	10759.0
177.90	235.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

m/z	Abundance
36.00	1576.0
37.00	8563.0
38.00	8159.0
39.00	3666.0
39.90	1296.0
41.90	105.0
42.80	179.0
44.00	1762.0
45.00	1518.0
46.00	370.0
47.10	2594.0
47.90	1357.0
49.00	7402.0
50.00	33992.0
51.00	11193.0
52.00	518.0
53.00	337.0
53.90	183.0
55.00	537.0
56.00	2659.0
57.00	5195.0
57.90	266.0
59.10	103.0
60.00	1770.0
61.00	9316.0
62.00	8934.0
63.00	7868.0
64.00	1461.0
65.00	2010.0
66.10	226.0
67.10	431.0
68.00	18720.0
69.00	18656.0
70.00	1561.0
71.20	144.0
72.00	1077.0
73.00	7249.0
74.00	30976.0
75.00	90024.0
76.00	7867.0
76.90	942.0
77.90	684.0
78.90	6463.0
79.90	1707.0
80.90	6327.0
81.90	1437.0
83.00	137.0
86.00	341.0
87.00	8148.0
87.90	7747.0
90.90	700.0
92.00	5080.0
93.00	8061.0
94.00	22416.0
95.00	181568.0
96.00	11913.0
97.00	354.0
102.70	101.0
103.80	808.0
104.90	321.0
105.90	926.0
106.70	201.0
108.10	173.0
110.00	190.0
110.80	232.0
112.00	209.0
112.90	222.0
114.90	328.0
115.90	535.0
116.90	1456.0
117.90	690.0
118.90	1370.0
123.80	179.0
127.80	706.0
128.90	332.0
129.90	774.0
130.80	295.0
134.80	352.0
136.70	251.0
139.90	180.0
140.90	1726.0
142.00	268.0
142.90	3032.0
143.80	202.0
144.90	1062.0
145.80	453.0
146.80	158.0
147.90	445.0
148.80	112.0
149.80	316.0
151.70	134.0
152.80	189.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

153.80	119.0
154.20	132.0
154.90	610.0
156.90	443.0
159.00	336.0
160.80	266.0
170.80	500.0
171.90	2966.0
173.00	1861.0
173.90	164928.0
174.90	12299.0
175.90	159680.0
176.90	9873.0
177.90	212.0
206.80	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

Scan 2793 (10.071 min): VV012824.D
BFB38

m/z	Abundance
36.10	158.0
40.00	1039.0
42.10	119.0
43.90	903.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38