

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091620\
 Data File : VV018234.D
 Acq On : 16 Sep 2020 13:55
 Operator : SY/MD
 Sample : L4012-14DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWT2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	88	rVB	192370	193296	15.56%	1.914%
2	1.579	145	152	163	rBV	154469	171958	13.84%	1.702%
3	2.122	310	321	355	rVB	321091	489790	39.43%	4.849%
4	2.399	402	407	410	rBV4	310	334	0.03%	0.003%
5	2.524	438	446	457	rVB2	4098	6898	0.56%	0.068%
6	2.585	463	465	470	rVB2	158	111	0.01%	0.001%
7	2.666	487	490	495	rVB	158	142	0.01%	0.001%
8	2.762	513	520	524	rBV	129	170	0.01%	0.002%
9	2.907	561	565	570	rBV	187	136	0.01%	0.001%
10	2.965	579	583	585	rBV2	125	106	0.01%	0.001%
11	3.074	613	617	620	rBV	174	164	0.01%	0.002%
12	3.126	625	633	641	rVB	176	316	0.03%	0.003%
13	3.171	641	647	649	rBV2	123	135	0.01%	0.001%
14	3.238	664	668	672	rVB	141	133	0.01%	0.001%
15	3.347	699	702	709	rVB2	115	132	0.01%	0.001%
16	3.527	752	758	761	rVV	92	99	0.01%	0.001%
17	3.585	770	776	778	rBV2	126	130	0.01%	0.001%
18	3.659	794	799	804	rVB2	156	157	0.01%	0.002%
19	3.740	820	824	828	rVB2	123	122	0.01%	0.001%
20	3.765	828	832	834	rBV2	153	118	0.01%	0.001%
21	3.807	840	845	848	rBV2	106	97	0.01%	0.001%
22	3.917	867	879	921	rBV	77731	252270	20.31%	2.497%
23	4.376	1005	1022	1048	rBV	196332	480659	38.70%	4.758%
24	4.534	1068	1071	1073	rBV2	324	164	0.01%	0.002%
25	4.569	1079	1082	1087	rVB4	261	290	0.02%	0.003%
26	4.698	1119	1122	1127	rVB	127	99	0.01%	0.001%
27	5.074	1216	1239	1265	rBV2	491636	1242095	100.00%	12.296%
28	5.306	1307	1311	1313	rBV2	216	103	0.01%	0.001%
29	5.389	1335	1337	1342	rVB	167	103	0.01%	0.001%
30	5.418	1342	1346	1349	rBV3	174	133	0.01%	0.001%
31	5.437	1349	1352	1356	rVB3	318	234	0.02%	0.002%
32	5.515	1373	1376	1383	rVB3	249	242	0.02%	0.002%
33	5.643	1402	1416	1445	rBV	301980	602089	48.47%	5.961%
34	5.791	1460	1462	1465	rVB2	358	187	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091620\
 Data File : VV018234.D
 Acq On : 16 Sep 2020 13:55
 Operator : SY/MD
 Sample : L4012-14DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWT2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

35	5.939	1495	1508	1539	rBV	546493	1071344	86.25%	10.606%
36	6.093	1543	1556	1581	rVV	275366	550713	44.34%	5.452%
37	6.238	1594	1601	1603	rBV4	500	559	0.05%	0.006%
38	6.280	1612	1614	1620	rVB3	403	298	0.02%	0.003%
39	6.492	1677	1680	1683	rBV2	145	102	0.01%	0.001%
40	6.518	1685	1688	1696	rVB2	152	180	0.01%	0.002%
41	6.560	1696	1701	1703	rBV	175	145	0.01%	0.001%
42	6.621	1717	1720	1725	rVB	168	149	0.01%	0.001%
43	6.653	1727	1730	1736	rBV2	88	116	0.01%	0.001%
44	6.701	1740	1745	1748	rVB2	123	120	0.01%	0.001%
45	6.939	1810	1819	1822	rBV2	138	151	0.01%	0.001%
46	7.010	1828	1841	1862	rBV	156598	280544	22.59%	2.777%
47	7.199	1897	1900	1904	rVB2	406	316	0.03%	0.003%
48	7.267	1918	1921	1923	rBV	228	127	0.01%	0.001%
49	7.338	1929	1943	1973	rBV	588309	1013447	81.59%	10.033%
50	7.643	2027	2038	2062	rBV	114281	197155	15.87%	1.952%
51	7.820	2091	2093	2096	rVB	242	98	0.01%	0.001%
52	7.875	2106	2110	2112	rBV2	176	126	0.01%	0.001%
53	7.913	2120	2122	2125	rVB3	196	104	0.01%	0.001%
54	7.965	2131	2138	2142	rBV2	317	464	0.04%	0.005%
55	8.106	2172	2182	2221	rBV	301736	517428	41.66%	5.122%
56	8.363	2259	2262	2270	rVB3	301	398	0.03%	0.004%
57	8.453	2287	2290	2292	rBV2	180	130	0.01%	0.001%
58	8.537	2313	2316	2318	rBV2	155	106	0.01%	0.001%
59	8.746	2377	2381	2384	rVB	159	122	0.01%	0.001%
60	8.820	2401	2404	2409	rBV2	138	124	0.01%	0.001%
61	8.875	2409	2421	2444	rBV	473179	758886	61.10%	7.513%
62	9.058	2474	2478	2481	rVB3	139	111	0.01%	0.001%
63	9.080	2481	2485	2488	rVB2	182	130	0.01%	0.001%
64	9.112	2492	2495	2500	rVB2	158	119	0.01%	0.001%
65	9.248	2534	2537	2544	rVB	172	163	0.01%	0.002%
66	9.280	2544	2547	2553	rBV	124	122	0.01%	0.001%
67	9.508	2615	2618	2623	rBV2	127	97	0.01%	0.001%
68	9.794	2704	2707	2711	rVB2	163	124	0.01%	0.001%
69	9.858	2723	2727	2732	rBV2	134	148	0.01%	0.001%
70	10.238	2832	2845	2861	rBV	368168	569973	45.89%	5.643%
71	10.318	2868	2870	2873	rBV	145	97	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091620\
 Data File : VV018234.D
 Acq On : 16 Sep 2020 13:55
 Operator : SY/MD
 Sample : L4012-14DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWT2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

72	10.376	2885	2888	2892	rVB2	176	132	0.01%	0.001%
73	10.399	2892	2895	2897	rBV	332	220	0.02%	0.002%
74	10.473	2916	2918	2923	rVB2	170	126	0.01%	0.001%
75	10.566	2944	2947	2950	rVB2	158	107	0.01%	0.001%
76	10.601	2955	2958	2964	rBV3	379	301	0.02%	0.003%
77	10.685	2981	2984	2989	rBV	98	105	0.01%	0.001%
78	10.791	3013	3017	3021	rBV	161	174	0.01%	0.002%
79	11.135	3120	3124	3131	rBV	198	225	0.02%	0.002%
80	11.167	3131	3134	3137	rBV2	166	132	0.01%	0.001%
81	11.206	3144	3146	3154	rVB3	301	228	0.02%	0.002%
82	11.270	3154	3166	3187	rBV	486508	735046	59.18%	7.277%
83	11.537	3246	3249	3256	rVB2	144	155	0.01%	0.002%
84	11.569	3256	3259	3261	rBV	143	102	0.01%	0.001%
85	11.646	3271	3283	3305	rBV	617951	953677	76.78%	9.441%
86	12.000	3390	3393	3397	rVB	175	131	0.01%	0.001%
87	12.167	3439	3445	3448	rBV	183	209	0.02%	0.002%
88	12.595	3571	3578	3581	rBV	178	212	0.02%	0.002%
89	12.681	3600	3605	3608	rBV2	199	196	0.02%	0.002%
90	12.730	3616	3620	3623	rBV2	163	167	0.01%	0.002%
91	13.296	3792	3796	3799	rBV3	369	295	0.02%	0.003%
92	13.624	3895	3898	3901	rBV2	145	121	0.01%	0.001%
93	13.691	3916	3919	3922	rBV	234	206	0.02%	0.002%
94	13.775	3942	3945	3950	rVB2	426	274	0.02%	0.003%
95	13.813	3954	3957	3959	rBV2	209	99	0.01%	0.001%
96	13.884	3976	3979	3983	rBV2	286	258	0.02%	0.003%
97	14.090	4041	4043	4047	rVB	302	166	0.01%	0.002%
98	14.128	4053	4055	4060	rVB	207	116	0.01%	0.001%
99	14.177	4068	4070	4072	rBV	210	106	0.01%	0.001%
100	14.482	4162	4165	4167	rBV	289	208	0.02%	0.002%


Sum of corrected areas: 10101242

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091620\
Data File : VV018234.D
Acq On : 16 Sep 2020 13:55
Operator : SY/MD
Sample : L4012-14DL 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWT2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

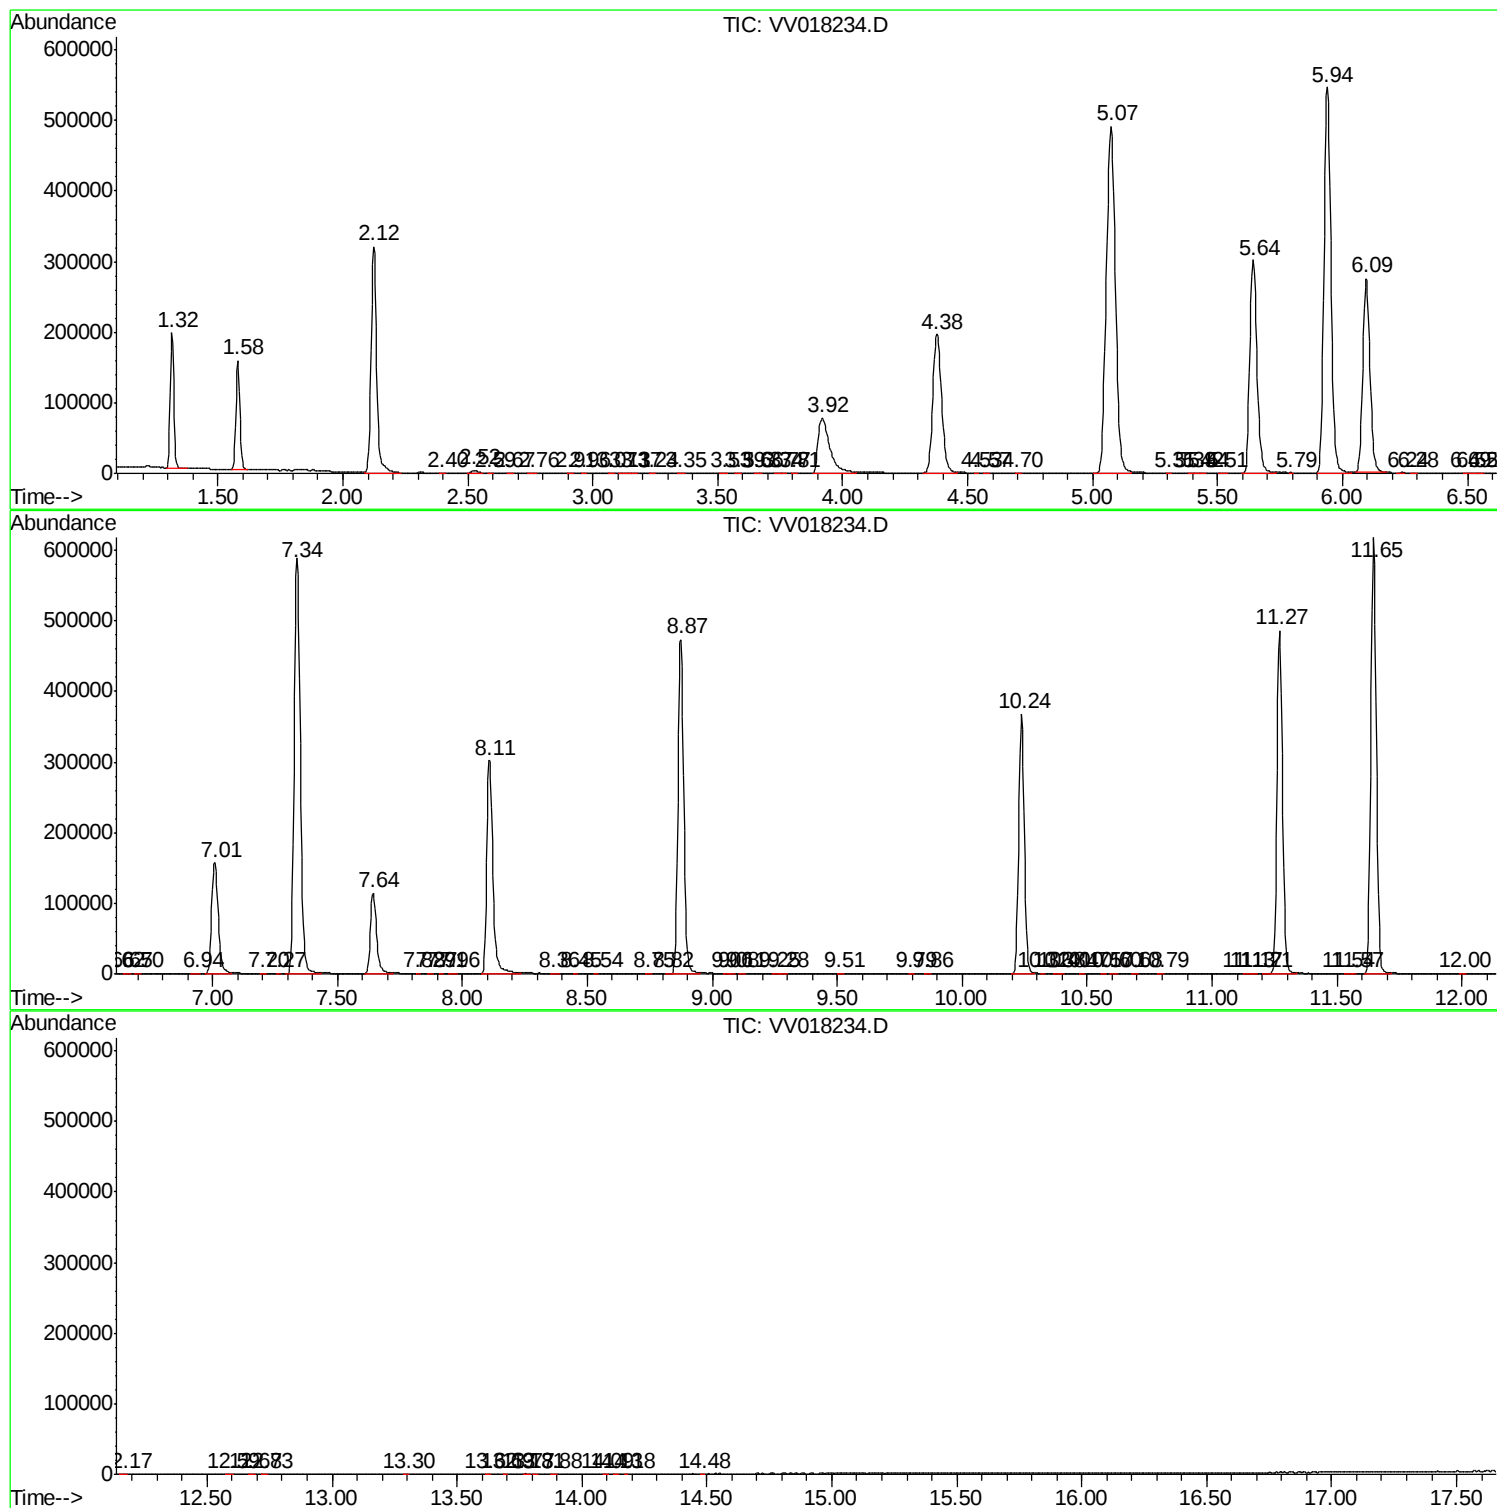

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV091620\
Data File : VV018234.D
Acq On : 16 Sep 2020 13:55
Operator : SY/MD
Sample : L4012-14DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWT2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091620\
Data File : VV018234.D
Acq On : 16 Sep 2020 13:55
Operator : SY/MD
Sample : L4012-14DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWT2DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc