

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091620\
 Data File : VV018261.D
 Acq On : 17 Sep 2020 01:35
 Operator : SY/MD
 Sample : L4042-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	147714	146870	15.04%	1.882%
2	1.579	145	152	168	rVB	117813	133961	13.72%	1.717%
3	2.122	311	321	363	rVB	251736	393194	40.26%	5.039%
4	2.656	484	487	490	rBV	120	65	0.01%	0.001%
5	2.688	494	497	499	rBV	116	77	0.01%	0.001%
6	2.737	509	512	513	rBV2	111	61	0.01%	0.001%
7	2.820	534	538	541	rBV	167	124	0.01%	0.002%
8	2.981	584	588	592	rBV2	121	138	0.01%	0.002%
9	3.119	623	631	633	rBV2	120	157	0.02%	0.002%
10	3.212	650	660	661	rBV2	1444	1550	0.16%	0.020%
11	3.470	737	740	742	rBV	96	58	0.01%	0.001%
12	3.502	747	750	756	rVV	103	94	0.01%	0.001%
13	3.531	756	759	761	rBV	71	49	0.01%	0.001%
14	3.679	801	805	806	rBV2	43	28	0.00%	0.000%
15	3.727	817	820	821	rBV	71	40	0.00%	0.001%
16	3.749	825	827	830	rVB	91	52	0.01%	0.001%
17	3.775	830	835	844	rBV2	139	183	0.02%	0.002%
18	3.849	856	858	859	rBV	29	14	0.00%	0.000%
19	3.875	863	866	868	rVB	94	46	0.00%	0.001%
20	3.926	868	882	918	rBV2	72118	257569	26.37%	3.301%
21	4.376	1005	1022	1050	rBV	156688	387088	39.64%	4.960%
22	4.563	1077	1080	1083	rBV	194	156	0.02%	0.002%
23	4.579	1083	1085	1092	rVV3	211	223	0.02%	0.003%
24	4.640	1092	1104	1117	rVV4	3076	6808	0.70%	0.087%
25	4.798	1151	1153	1154	rBV	61	29	0.00%	0.000%
26	4.843	1164	1167	1168	rBV2	74	42	0.00%	0.001%
27	4.878	1174	1178	1181	rBV2	120	95	0.01%	0.001%
28	4.984	1209	1211	1212	rBV	50	25	0.00%	0.000%
29	5.074	1221	1239	1269	rBV2	386270	976616	100.00%	12.515%
30	5.277	1297	1302	1305	rBV3	269	253	0.03%	0.003%
31	5.386	1333	1336	1338	rVB2	53	27	0.00%	0.000%
32	5.408	1339	1343	1345	rBV2	148	103	0.01%	0.001%
33	5.434	1350	1351	1352	rVB2	124	24	0.00%	0.000%
34	5.447	1352	1355	1362	rBV2	222	166	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091620\
 Data File : VV018261.D
 Acq On : 17 Sep 2020 01:35
 Operator : SY/MD
 Sample : L4042-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

35	5.508	1372	1374	1375	rBV	102	39	0.00%	0.000%
36	5.643	1403	1416	1442	rBV	334716	667507	68.35%	8.554%
37	5.942	1499	1509	1523	rVB8	4442	9938	1.02%	0.127%
38	6.013	1528	1531	1533	rBV	60	34	0.00%	0.000%
39	6.039	1534	1539	1543	rBV2	169	216	0.02%	0.003%
40	6.093	1543	1556	1581	rBV	215294	437792	44.83%	5.610%
41	6.238	1597	1601	1603	rBV2	430	299	0.03%	0.004%
42	6.280	1611	1614	1621	rVB2	122	106	0.01%	0.001%
43	6.312	1621	1624	1627	rBV2	88	76	0.01%	0.001%
44	6.360	1636	1639	1642	rBV2	53	36	0.00%	0.000%
45	6.379	1642	1645	1649	rBV2	107	78	0.01%	0.001%
46	6.447	1662	1666	1669	rBV	108	109	0.01%	0.001%
47	6.540	1690	1695	1697	rBV2	96	88	0.01%	0.001%
48	6.553	1697	1699	1702	rVB2	98	47	0.00%	0.001%
49	6.585	1706	1709	1713	rBV2	72	50	0.01%	0.001%
50	6.617	1714	1719	1723	rBV2	72	93	0.01%	0.001%
51	6.682	1736	1739	1741	rBV2	102	51	0.01%	0.001%
52	6.701	1741	1745	1746	rBV	53	41	0.00%	0.001%
53	6.752	1756	1761	1763	rBV	69	68	0.01%	0.001%
54	6.833	1784	1786	1790	rVB	80	61	0.01%	0.001%
55	6.852	1790	1792	1794	rBV	50	28	0.00%	0.000%
56	6.865	1794	1796	1798	rVB	49	21	0.00%	0.000%
57	6.881	1798	1801	1803	rBV	127	71	0.01%	0.001%
58	6.958	1822	1825	1826	rBV	45	21	0.00%	0.000%
59	7.010	1829	1841	1873	rBV	115133	209543	21.46%	2.685%
60	7.174	1889	1892	1894	rBV2	142	125	0.01%	0.002%
61	7.190	1896	1897	1905	rVB2	300	198	0.02%	0.003%
62	7.257	1913	1918	1922	rBB	89	80	0.01%	0.001%
63	7.338	1931	1943	1968	rBV	447576	770275	78.87%	9.871%
64	7.595	2019	2023	2024	rBV2	120	70	0.01%	0.001%
65	7.643	2028	2038	2062	rBV	85348	146514	15.00%	1.878%
66	7.839	2096	2099	2101	rBV2	117	70	0.01%	0.001%
67	7.881	2108	2112	2114	rBV2	84	66	0.01%	0.001%
68	7.910	2118	2121	2123	rBV	89	51	0.01%	0.001%
69	7.926	2123	2126	2130	rVB	110	62	0.01%	0.001%
70	7.952	2130	2134	2135	rBV	128	66	0.01%	0.001%
71	7.994	2144	2147	2151	rBV2	75	67	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091620\
 Data File : VV018261.D
 Acq On : 17 Sep 2020 01:35
 Operator : SY/MD
 Sample : L4042-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

72	8.109	2173	2183	2211	rBV	240342	412604	42.25%	5.287%
73	8.431	2278	2283	2286	rBV2	283	312	0.03%	0.004%
74	8.482	2297	2299	2302	rVB2	177	81	0.01%	0.001%
75	8.611	2336	2339	2340	rBV2	76	44	0.00%	0.001%
76	8.656	2349	2353	2356	rBV	206	140	0.01%	0.002%
77	8.694	2362	2365	2366	rBV	206	79	0.01%	0.001%
78	8.775	2386	2390	2392	rBV2	93	72	0.01%	0.001%
79	8.875	2408	2421	2448	rBV	528077	841518	86.17%	10.784%
80	9.347	2564	2568	2571	rBV2	145	120	0.01%	0.002%
81	9.395	2578	2583	2588	rBV2	187	171	0.02%	0.002%
82	9.810	2709	2712	2716	rVB	91	63	0.01%	0.001%
83	9.839	2716	2721	2723	rBV	161	124	0.01%	0.002%
84	10.238	2832	2845	2861	rBV	293197	456913	46.79%	5.855%
85	10.350	2876	2880	2884	rBV2	120	135	0.01%	0.002%
86	10.399	2890	2895	2898	rBV3	272	324	0.03%	0.004%
87	10.849	3032	3035	3037	rBV	102	70	0.01%	0.001%
88	10.878	3042	3044	3046	rVV2	133	36	0.00%	0.000%
89	11.100	3109	3113	3116	rBV2	192	173	0.02%	0.002%
90	11.270	3155	3166	3192	rBV	519619	797336	81.64%	10.218%
91	11.434	3214	3217	3219	rBV	246	160	0.02%	0.002%
92	11.559	3251	3256	3259	rBV2	342	376	0.04%	0.005%
93	11.646	3271	3283	3302	rBV	480788	742129	75.99%	9.510%
94	11.797	3327	3330	3331	rBV2	225	108	0.01%	0.001%
95	11.868	3348	3352	3355	rBV3	315	227	0.02%	0.003%
96	12.032	3400	3403	3406	rBV2	175	151	0.02%	0.002%
97	13.186	3760	3762	3766	rBV2	158	81	0.01%	0.001%


Sum of corrected areas: 7803589

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091620\
Data File : VV018261.D
Acq On : 17 Sep 2020 01:35
Operator : SY/MD
Sample : L4042-15
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

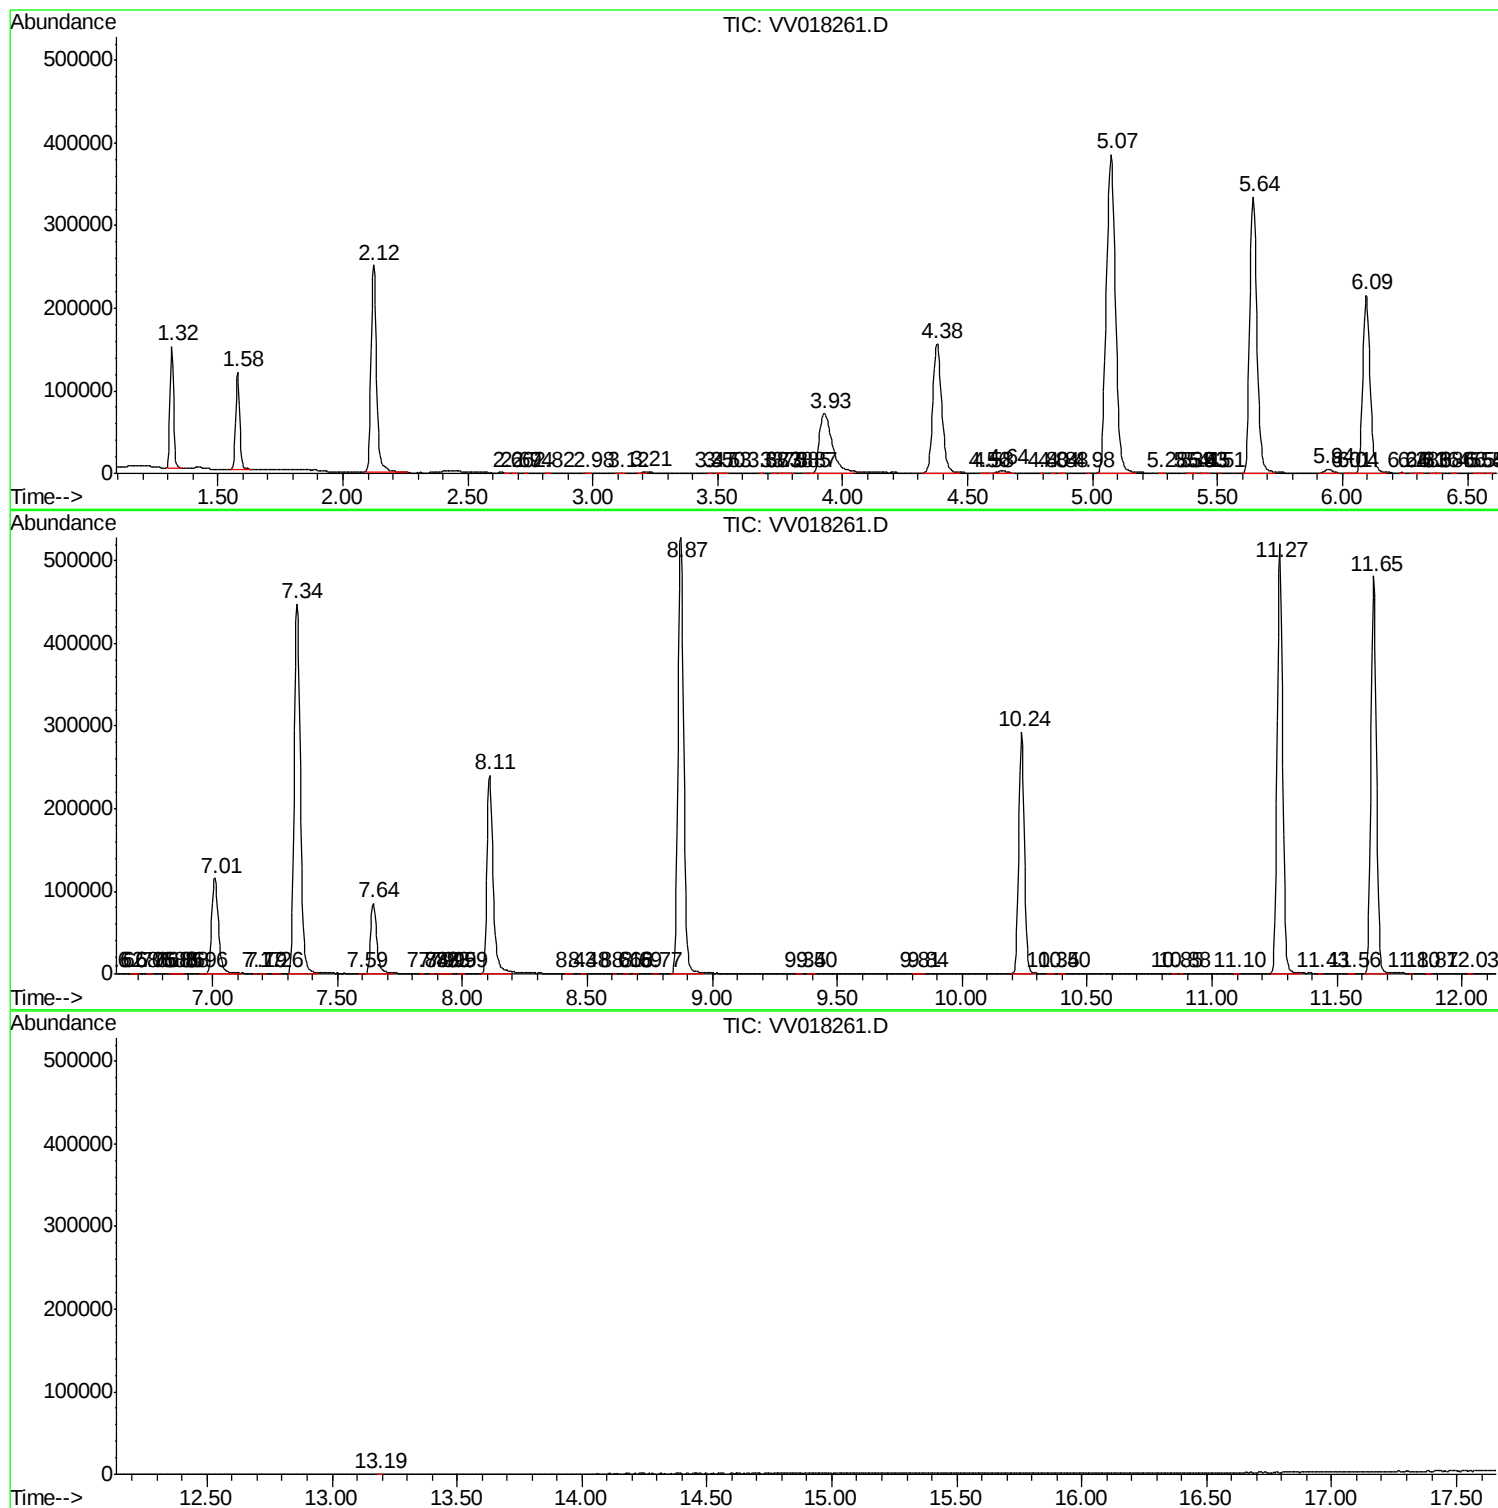

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV091620\
Data File : VV018261.D
Acq On : 17 Sep 2020 01:35
Operator : SY/MD
Sample : L4042-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091620\
Data File : VV018261.D
Acq On : 17 Sep 2020 01:35
Operator : SY/MD
Sample : L4042-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc