

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091621\
 Data File : VV022156.D
 Acq On : 16 Sep 2021 14:56
 Operator : SY/MD
 Sample : M3764-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C90

Quant Time: Sep 17 01:56:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 17 01:54:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	293819	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	281864	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	125859	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	91618	45.027	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	90.060%
7) Chloroethane-d5	1.561	69	79456	50.004	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	100.000%
11) 1,1-Dichloroethene-d2	2.104	63	136565	40.583	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.160%
21) 2-Butanone-d5	3.873	46	159010	113.948	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	113.950%
24) Chloroform-d	4.352	84	195528	52.701	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.400%
26) 1,2-Dichloroethane-d4	5.034	65	120608	55.190	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	110.380%
32) Benzene-d6	5.050	84	399673	52.278	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.560%
36) 1,2-Dichloropropane-d6	6.072	67	126635	52.671	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	105.340%
41) Toluene-d8	7.316	98	354285	49.092	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.180%
43) trans-1,3-Dichloroprop...	7.625	79	54648	47.755	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.500%
47) 2-Hexanone-d5	8.088	63	100124	108.533	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	108.530%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	166652	54.121	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	108.240%
66) 1,2-Dichlorobenzene-d4	11.625	152	137612	55.618	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	111.240%
Target Compounds						
12) 1,1-Dichloroethene	2.108	96	1704	1.005	ug/L	Qvalue # 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091621\
Data File : VV022156.D
Acq On : 16 Sep 2021 14:56
Operator : SY/MD
Sample : M3764-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C90


Quant Time: Sep 17 01:56:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 17 01:54:12 2021
Response via : Initial Calibration

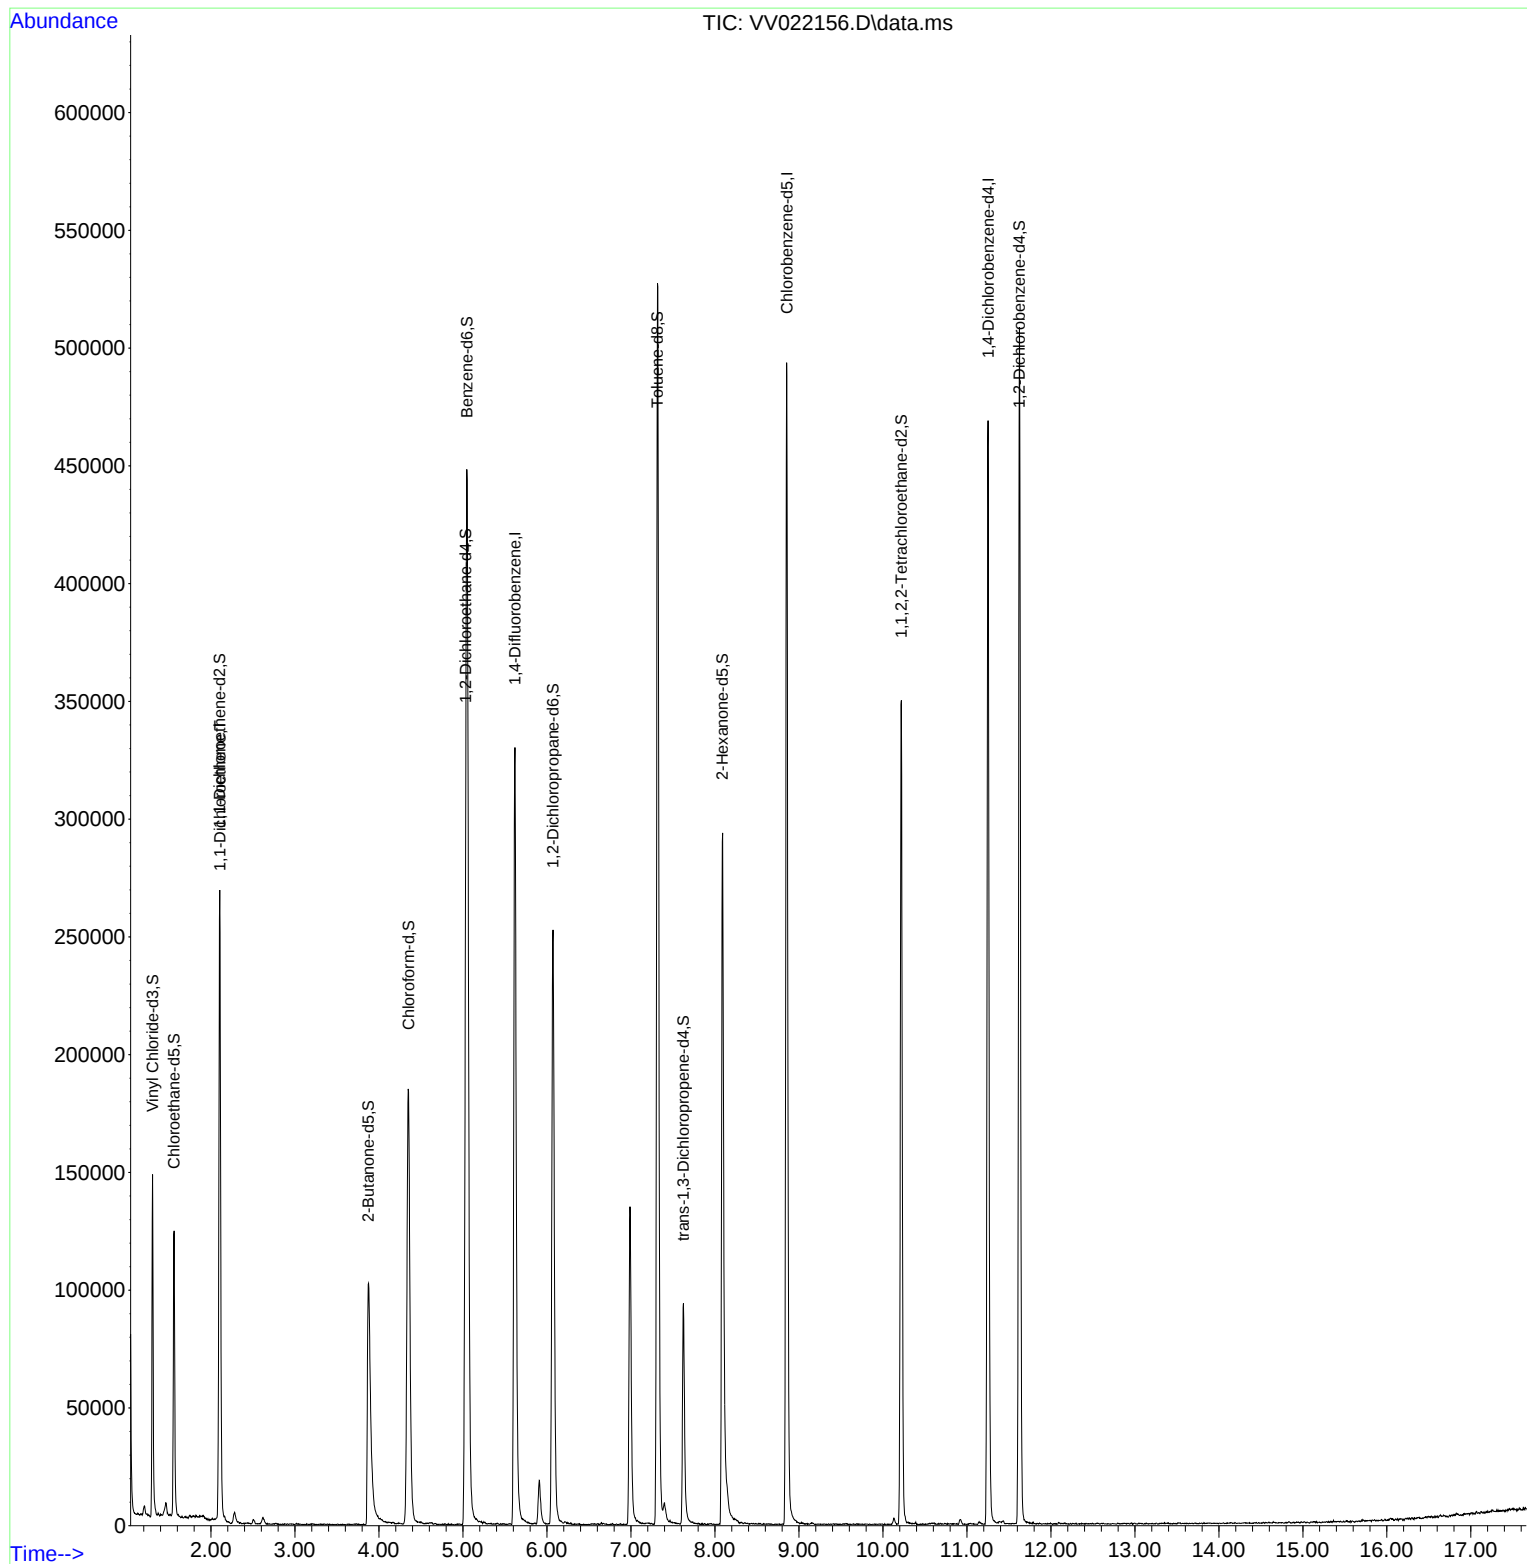

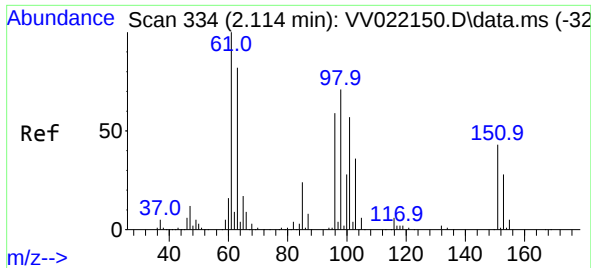

#12
 1,1-Dichloroethene
 Concen: 1.005 ug/L
 RT: 2.108 min Scan# 332
 Delta R.T. -0.007 min
 Lab File: VV022156.D
 Acq: 16 Sep 2021 14:56

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C90

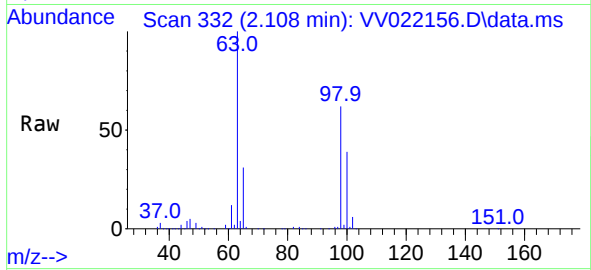

Tgt Ion: 96 Resp: 1704
 Ion Ratio Lower Upper
 96 100
 61 1090.9 113.2 210.2#
 63 8768.6 102.3 189.9#

