

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091621\
 Data File : VV022162.D
 Acq On : 16 Sep 2021 17:44
 Operator : SY/MD
 Sample : M3764-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C99

Quant Time: Sep 17 01:57:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 17 01:54:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	308317	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	291031	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	128870	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	93753	43.910	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.820%
7) Chloroethane-d5	1.564	69	79758	47.834	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.660%
11) 1,1-Dichloroethene-d2	2.104	63	138131	39.118	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.240%
21) 2-Butanone-d5	3.899	46	169169	115.528	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	115.530%
24) Chloroform-d	4.352	84	194570	49.977	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.960%
26) 1,2-Dichloroethane-d4	5.034	65	122497	53.418	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.840%
32) Benzene-d6	5.053	84	397102	50.306	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.620%
36) 1,2-Dichloropropane-d6	6.072	67	128259	51.666	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.340%
41) Toluene-d8	7.317	98	355563	47.717	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.440%
43) trans-1,3-Dichloroprop...	7.625	79	53143	44.977	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.960%
47) 2-Hexanone-d5	8.091	63	104056	109.243	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	109.240%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	162589	51.139	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	102.280%
66) 1,2-Dichlorobenzene-d4	11.625	152	134764	53.194	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.380%
Target Compounds						
12) 1,1-Dichloroethene	2.111	96	2714	1.526	ug/L	Qvalue # 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091621\
Data File : VV022162.D
Acq On : 16 Sep 2021 17:44
Operator : SY/MD
Sample : M3764-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C99


Quant Time: Sep 17 01:57:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 17 01:54:12 2021
Response via : Initial Calibration

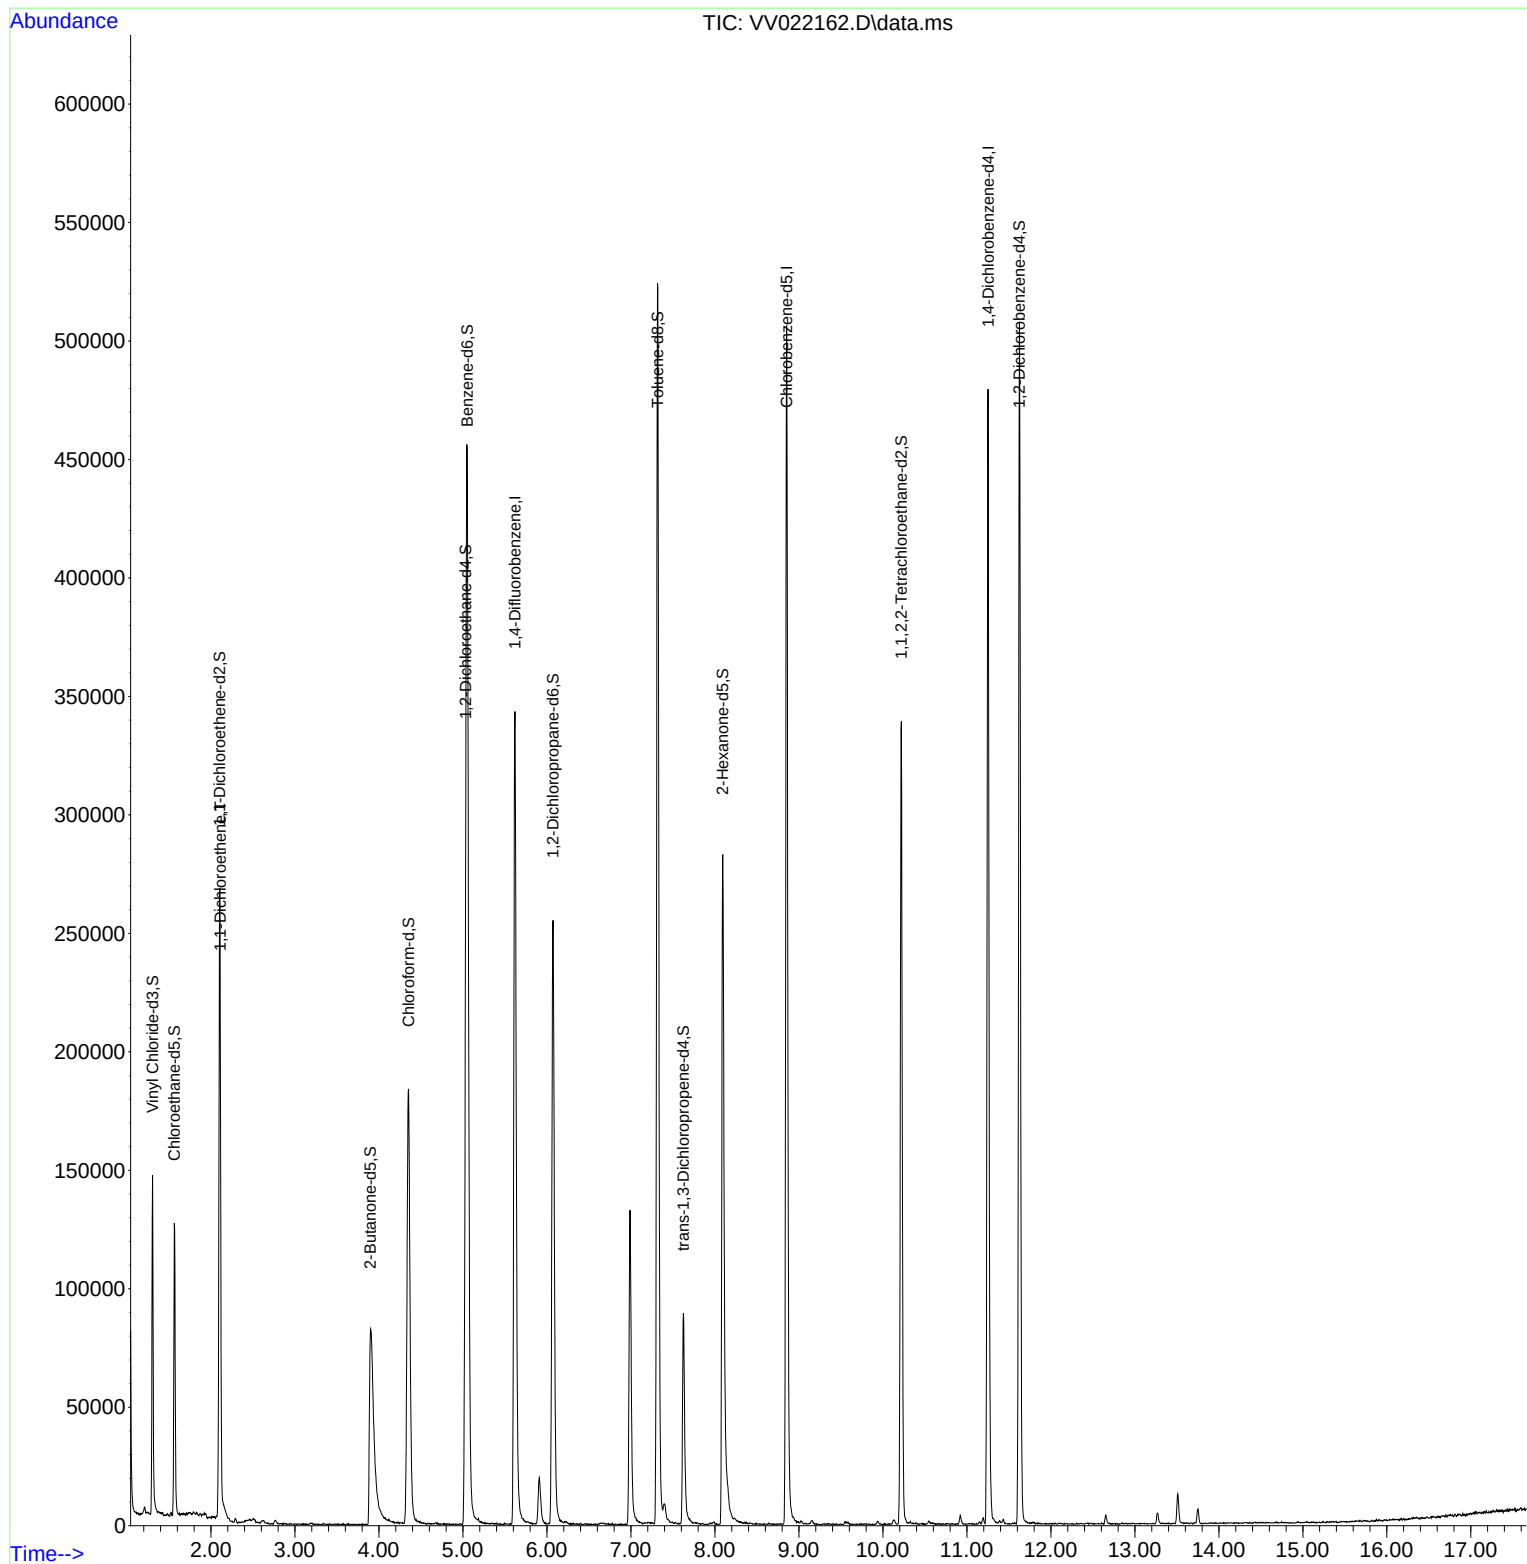

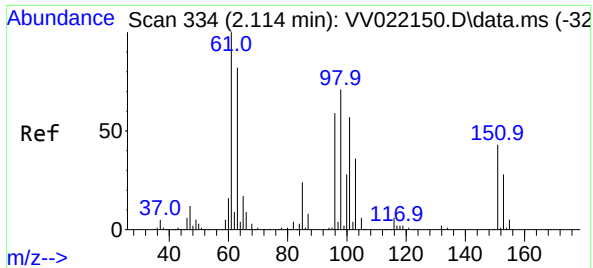

#12
1,1-Dichloroethene
Concen: 1.526 ug/L
RT: 2.111 min Scan# 333
Delta R.T. -0.003 min
Lab File: VV022162.D
Acq: 16 Sep 2021 17:44

Instrument :
MSVOA_V
ClientSampleId :
C0C99

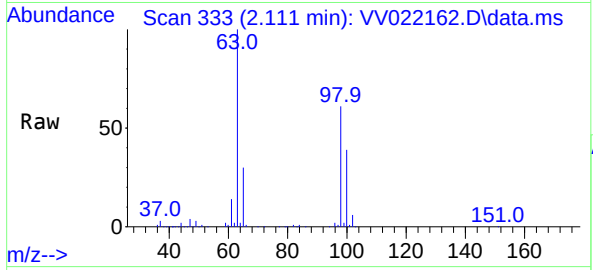

Tgt Ion: 96 Resp: 2714
Ion Ratio Lower Upper
96 100
61 685.5 113.2 210.2#
63 4950.7 102.3 189.9#

