

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091621\
 Data File : VV022155.D
 Acq On : 16 Sep 2021 14:31
 Operator : SY/MD
 Sample : M3764-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022155.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rBV	148397	151654	13.04%	1.710%
2	1.561	154	162	177	rBV	131083	153187	13.17%	1.727%
3	2.105	321	331	358	rVB	274921	411788	35.41%	4.644%
4	2.384	416	418	422	rVB2	524	225	0.02%	0.003%
5	2.407	422	425	430	rBV4	515	539	0.05%	0.006%
6	2.429	430	432	434	rBV2	502	254	0.02%	0.003%
7	2.510	449	457	467	rVB6	2091	3367	0.29%	0.038%
8	2.561	467	473	476	rVB2	437	451	0.04%	0.005%
9	2.757	531	534	537	rBV	506	342	0.03%	0.004%
10	2.796	544	546	551	rVB3	344	235	0.02%	0.003%
11	2.886	573	574	580	rVV	323	190	0.02%	0.002%
12	2.915	581	583	588	rVB4	487	378	0.03%	0.004%
13	2.966	596	599	606	rVB2	464	444	0.04%	0.005%
14	2.995	606	608	611	rBV2	180	110	0.01%	0.001%
15	3.105	638	642	647	rVB2	240	246	0.02%	0.003%
16	3.134	647	651	652	rBV	347	228	0.02%	0.003%
17	3.259	688	690	693	rBV	221	141	0.01%	0.002%
18	3.291	697	700	705	rVB	404	296	0.03%	0.003%
19	3.452	746	750	754	rVB3	247	206	0.02%	0.002%
20	3.478	754	758	760	rBV	223	151	0.01%	0.002%
21	3.513	766	769	771	rBV	163	113	0.01%	0.001%
22	3.539	773	777	779	rBV2	169	122	0.01%	0.001%
23	3.690	821	824	828	rBV	190	143	0.01%	0.002%
24	3.709	828	830	835	rVV	265	151	0.01%	0.002%
25	3.738	835	839	841	rVV2	134	114	0.01%	0.001%
26	3.764	844	847	852	rVB2	393	287	0.02%	0.003%
27	3.825	863	866	869	rVB2	361	176	0.02%	0.002%
28	3.876	872	882	917	rBV	103591	275290	23.67%	3.104%
29	4.349	1013	1029	1055	rBV	187290	461443	39.68%	5.204%
30	4.661	1122	1126	1128	rBV2	382	223	0.02%	0.003%
31	4.745	1151	1152	1154	rBV2	316	146	0.01%	0.002%
32	4.815	1173	1174	1181	rVB2	273	137	0.01%	0.002%
33	5.047	1229	1246	1270	rBV2	453727	1162993	100.00%	13.115%
34	5.269	1311	1315	1319	rBV4	426	500	0.04%	0.006%
35	5.410	1357	1359	1361	rBV	287	168	0.01%	0.002%
36	5.449	1370	1371	1373	rBV2	398	121	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091621\
 Data File : VV022155.D
 Acq On : 16 Sep 2021 14:31
 Operator : SY/MD
 Sample : M3764-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	5.490	1379	1384	1385	rBV2	309	245	0.02%	0.003%
38	5.619	1411	1424	1452	rBV	338658	684748	58.88%	7.722%
39	5.915	1500	1516	1536	rBV4	65210	151686	13.04%	1.711%
40	6.072	1551	1565	1594	rBV	254257	524704	45.12%	5.917%
41	6.314	1637	1640	1643	rBV2	437	320	0.03%	0.004%
42	6.371	1654	1658	1662	rBB2	277	241	0.02%	0.003%
43	6.391	1662	1664	1667	rVB	466	221	0.02%	0.002%
44	6.426	1671	1675	1678	rBV2	399	235	0.02%	0.003%
45	6.535	1706	1709	1714	rVB3	363	292	0.03%	0.003%
46	6.638	1736	1741	1744	rBV2	691	607	0.05%	0.007%
47	6.725	1765	1768	1774	rVB3	350	341	0.03%	0.004%
48	6.770	1778	1782	1784	rBV	237	174	0.01%	0.002%
49	6.863	1808	1811	1814	rBV	186	131	0.01%	0.001%
50	6.989	1838	1850	1877	rBV	136997	254402	21.87%	2.869%
51	7.317	1937	1952	1971	rBV	537633	937757	80.63%	10.575%
52	7.625	2038	2048	2072	rBV	93276	165104	14.20%	1.862%
53	7.867	2118	2123	2127	rBV3	364	342	0.03%	0.004%
54	7.934	2141	2144	2145	rBV	270	142	0.01%	0.002%
55	8.008	2165	2167	2172	rVB3	501	292	0.03%	0.003%
56	8.034	2172	2175	2178	rVB2	208	123	0.01%	0.001%
57	8.092	2182	2193	2224	rBV	295318	562418	48.36%	6.342%
58	8.519	2322	2326	2328	rBV2	451	327	0.03%	0.004%
59	8.564	2336	2340	2343	rBV2	354	307	0.03%	0.003%
60	8.664	2368	2371	2376	rVB2	289	219	0.02%	0.002%
61	8.728	2387	2391	2394	rVV2	264	229	0.02%	0.003%
62	8.783	2404	2408	2411	rVB2	358	227	0.02%	0.003%
63	8.802	2411	2414	2416	rBV2	205	121	0.01%	0.001%
64	8.854	2416	2430	2453	rBV	506284	822032	70.68%	9.270%
65	9.143	2517	2520	2523	rBV2	560	486	0.04%	0.005%
66	9.291	2562	2566	2570	rBV2	445	358	0.03%	0.004%
67	9.336	2578	2580	2586	rVB2	248	145	0.01%	0.002%
68	9.432	2607	2610	2612	rBV2	254	143	0.01%	0.002%
69	9.445	2612	2614	2617	rVB3	351	198	0.02%	0.002%
70	9.522	2637	2638	2644	rVB3	355	238	0.02%	0.003%
71	9.548	2644	2646	2647	rVV3	257	126	0.01%	0.001%
72	9.558	2647	2649	2655	rVV3	441	354	0.03%	0.004%
73	9.609	2662	2665	2669	rVB2	251	189	0.02%	0.002%
74	9.674	2679	2685	2687	rBV2	300	251	0.02%	0.003%
75	9.841	2734	2737	2739	rBV2	262	176	0.02%	0.002%
76	9.976	2776	2779	2782	rBB	282	161	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091621\
 Data File : VV022155.D
 Acq On : 16 Sep 2021 14:31
 Operator : SY/MD
 Sample : M3764-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0C88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.053	2800	2803	2809	rBV	305	226	0.02%	0.003%
78	10.130	2819	2827	2839	rVB7	2550	4359	0.37%	0.049%
79	10.217	2842	2854	2875	rBV	351784	553208	47.57%	6.239%
80	10.317	2882	2885	2887	rBV2	623	428	0.04%	0.005%
81	10.448	2924	2926	2931	rBV2	295	215	0.02%	0.002%
82	10.545	2954	2956	2957	rBV	311	121	0.01%	0.001%
83	10.580	2965	2967	2973	rBV5	641	494	0.04%	0.006%
84	10.976	3087	3090	3092	rBV	329	164	0.01%	0.002%
85	11.146	3138	3143	3152	rVB4	1083	1657	0.14%	0.019%
86	11.178	3152	3153	3156	rBV	228	118	0.01%	0.001%
87	11.214	3161	3164	3165	rBV	365	227	0.02%	0.003%
88	11.252	3165	3176	3197	rBV	481575	748317	64.34%	8.439%
89	11.474	3242	3245	3247	rBV	264	160	0.01%	0.002%
90	11.532	3259	3263	3266	rBV3	609	591	0.05%	0.007%
91	11.625	3281	3292	3314	rBV	518883	817460	70.29%	9.219%
92	11.947	3390	3392	3396	rVB2	335	201	0.02%	0.002%
93	12.182	3463	3465	3467	rBV	491	207	0.02%	0.002%
94	12.246	3482	3485	3489	rVB3	544	358	0.03%	0.004%
95	12.416	3536	3538	3543	rVB3	527	337	0.03%	0.004%
96	12.442	3543	3546	3549	rBV2	275	173	0.01%	0.002%
97	12.516	3567	3569	3572	rBV2	227	137	0.01%	0.002%
98	12.606	3596	3597	3604	rBV2	357	239	0.02%	0.003%
99	13.069	3739	3741	3745	rBV	299	246	0.02%	0.003%
100	13.480	3864	3869	3874	rVB3	570	560	0.05%	0.006%




Sum of corrected areas: 8867574

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091621\
Data File : VV022155.D
Acq On : 16 Sep 2021 14:31
Operator : SY/MD
Sample : M3764-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

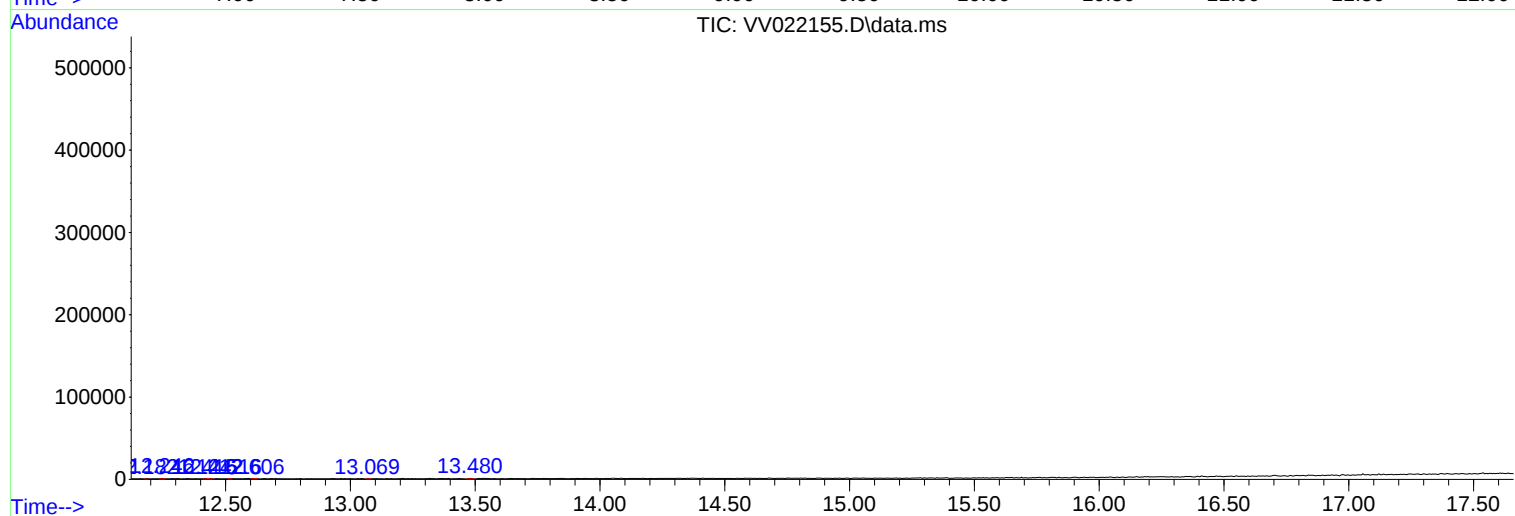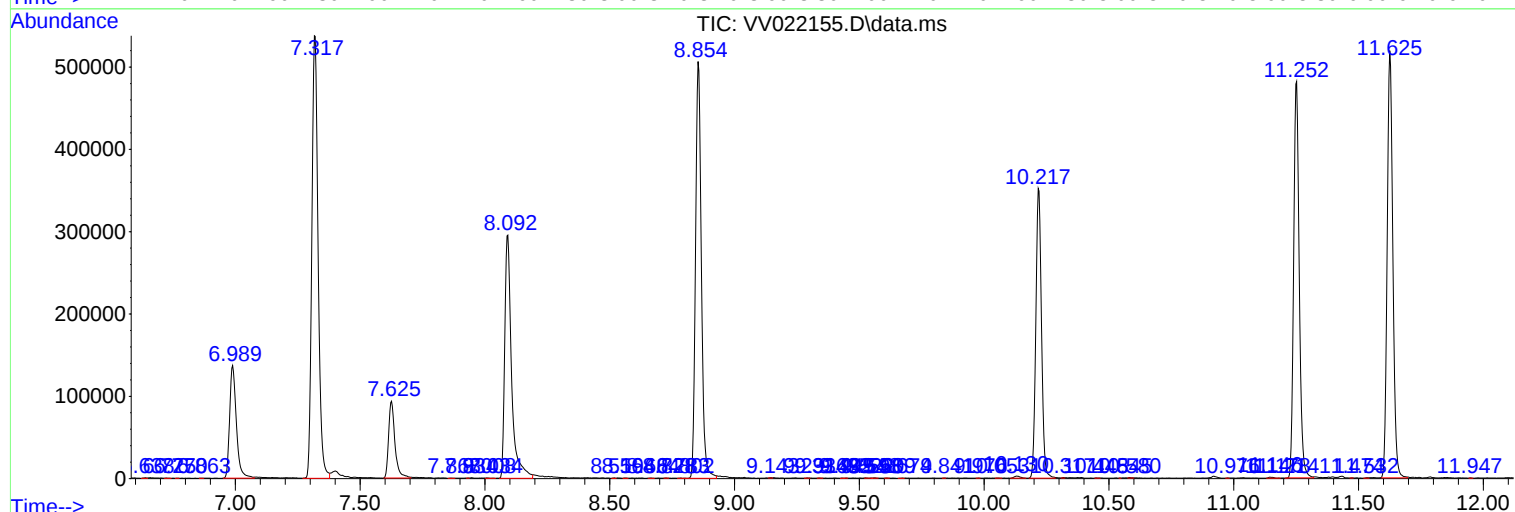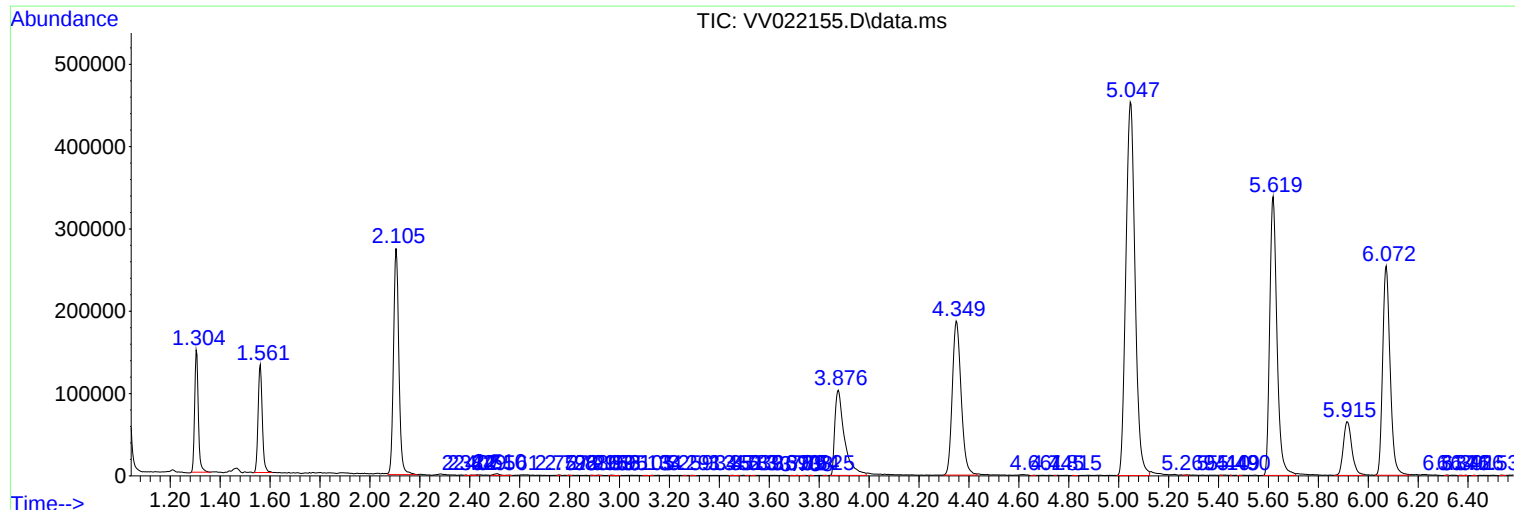

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091621\
Data File : VV022155.D
Acq On : 16 Sep 2021 14:31
Operator : SY/MD
Sample : M3764-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091621\
Data File : VV022155.D
Acq On : 16 Sep 2021 14:31
Operator : SY/MD
Sample : M3764-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0C88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
