

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091621\
 Data File : VV022163.D
 Acq On : 16 Sep 2021 18:09
 Operator : SY/MD
 Sample : M3764-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022163.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rBV	138216	141050	12.28%	1.628%
2	1.564	157	163	173	rBV	124997	138915	12.10%	1.603%
3	2.105	322	331	366	rVB	265413	399448	34.78%	4.610%
4	2.883	569	573	574	rBV2	472	272	0.02%	0.003%
5	2.905	577	580	583	rBV	330	239	0.02%	0.003%
6	2.963	594	598	603	rBV4	267	295	0.03%	0.003%
7	3.014	611	614	616	rBV	198	116	0.01%	0.001%
8	3.024	616	617	620	rVB	314	97	0.01%	0.001%
9	3.040	620	622	625	rVB2	306	163	0.01%	0.002%
10	3.059	625	628	629	rBV2	326	126	0.01%	0.001%
11	3.114	641	645	648	rBV3	441	290	0.03%	0.003%
12	3.223	677	679	682	rBV	310	205	0.02%	0.002%
13	3.394	730	732	735	rBV	172	83	0.01%	0.001%
14	3.458	749	752	761	rBV3	324	375	0.03%	0.004%
15	3.494	761	763	766	rVV	159	77	0.01%	0.001%
16	3.725	829	835	836	rBV	277	225	0.02%	0.003%
17	3.770	845	849	851	rBV2	285	175	0.02%	0.002%
18	3.895	877	888	925	rBV	88451	286153	24.92%	3.303%
19	4.349	1013	1029	1057	rBV	183156	457788	39.86%	5.284%
20	4.609	1108	1110	1112	rBV	288	141	0.01%	0.002%
21	4.686	1132	1134	1137	rVV2	398	207	0.02%	0.002%
22	4.719	1141	1144	1145	rBV2	190	105	0.01%	0.001%
23	4.757	1154	1156	1161	rBV2	252	206	0.02%	0.002%
24	4.850	1184	1185	1188	rBV2	269	155	0.01%	0.002%
25	4.899	1198	1200	1202	rVB	285	95	0.01%	0.001%
26	4.924	1206	1208	1211	rBV	171	106	0.01%	0.001%
27	4.969	1219	1222	1223	rBV	334	180	0.02%	0.002%
28	5.047	1229	1246	1277	rBV2	451526	1148399	100.00%	13.255%
29	5.336	1332	1336	1338	rBV4	516	329	0.03%	0.004%
30	5.403	1353	1357	1362	rVB3	538	321	0.03%	0.004%
31	5.429	1362	1365	1368	rVB3	348	234	0.02%	0.003%
32	5.448	1368	1371	1373	rBV2	389	209	0.02%	0.002%
33	5.526	1393	1395	1397	rVB2	194	82	0.01%	0.001%
34	5.538	1397	1399	1402	rBV	307	122	0.01%	0.001%
35	5.558	1402	1405	1406	rBV2	146	86	0.01%	0.001%
36	5.619	1411	1424	1456	rBV	343328	696564	60.66%	8.040%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091621\
 Data File : VV022163.D
 Acq On : 16 Sep 2021 18:09
 Operator : SY/MD
 Sample : M3764-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	5.915	1503	1516	1536	rBV5	42426	102118	8.89%	1.179%
38	6.014	1544	1547	1549	rBV	456	252	0.02%	0.003%
39	6.072	1552	1565	1587	rBV	252056	515834	44.92%	5.954%
40	6.288	1630	1632	1634	rBV	246	86	0.01%	0.001%
41	6.336	1644	1647	1650	rVB2	310	153	0.01%	0.002%
42	6.352	1650	1652	1658	rBV2	308	313	0.03%	0.004%
43	6.436	1675	1678	1682	rVB3	328	217	0.02%	0.003%
44	6.506	1698	1700	1701	rBV3	236	99	0.01%	0.001%
45	6.545	1709	1712	1713	rBV	261	132	0.01%	0.002%
46	6.728	1766	1769	1773	rBV2	265	236	0.02%	0.003%
47	6.747	1773	1775	1777	rVB2	392	190	0.02%	0.002%
48	6.789	1784	1788	1789	rBV2	246	167	0.01%	0.002%
49	6.876	1812	1815	1818	rBV	329	226	0.02%	0.003%
50	6.989	1838	1850	1878	rBV2	127673	241711	21.05%	2.790%
51	7.259	1931	1934	1936	rBV	476	325	0.03%	0.004%
52	7.320	1940	1953	1972	rBV	521080	906864	78.97%	10.467%
53	7.625	2036	2048	2069	rBV	89624	157936	13.75%	1.823%
54	7.866	2117	2123	2126	rBV4	572	442	0.04%	0.005%
55	7.915	2135	2138	2140	rBV	292	166	0.01%	0.002%
56	7.982	2154	2159	2163	rBV2	409	341	0.03%	0.004%
57	8.030	2171	2174	2177	rBV	617	314	0.03%	0.004%
58	8.091	2183	2193	2231	rBV	285563	568483	49.50%	6.561%
59	8.493	2314	2318	2321	rBV2	346	252	0.02%	0.003%
60	8.567	2339	2341	2342	rBV	289	131	0.01%	0.002%
61	8.593	2346	2349	2351	rBV2	166	133	0.01%	0.002%
62	8.706	2382	2384	2387	rVB3	519	199	0.02%	0.002%
63	8.757	2395	2400	2404	rVB2	635	426	0.04%	0.005%
64	8.783	2404	2408	2411	rBV2	552	344	0.03%	0.004%
65	8.853	2419	2430	2454	rBV	506408	825571	71.89%	9.529%
66	9.191	2534	2535	2537	rBV	364	96	0.01%	0.001%
67	9.217	2539	2543	2544	rBV	160	130	0.01%	0.002%
68	9.271	2558	2560	2563	rVB2	157	78	0.01%	0.001%
69	9.307	2569	2571	2574	rBV2	311	161	0.01%	0.002%
70	9.400	2598	2600	2604	rBV	277	206	0.02%	0.002%
71	9.419	2604	2606	2607	rBV	224	85	0.01%	0.001%
72	9.490	2625	2628	2631	rBV2	205	116	0.01%	0.001%
73	9.542	2643	2644	2645	rBV	282	98	0.01%	0.001%
74	9.583	2654	2657	2659	rBV2	418	227	0.02%	0.003%
75	9.664	2679	2682	2686	rBV3	298	259	0.02%	0.003%
76	9.699	2690	2693	2696	rBV	399	245	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091621\
 Data File : VV022163.D
 Acq On : 16 Sep 2021 18:09
 Operator : SY/MD
 Sample : M3764-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	9.818	2727	2730	2734	rVB3	416	251	0.02%	0.003%
78	9.988	2780	2783	2785	rBV	216	147	0.01%	0.002%
79	10.027	2792	2795	2798	rBV2	356	225	0.02%	0.003%
80	10.130	2819	2827	2835	rBV6	2032	3456	0.30%	0.040%
81	10.217	2842	2854	2874	rBV	329546	530719	46.21%	6.126%
82	10.506	2941	2944	2947	rBV3	387	262	0.02%	0.003%
83	10.628	2980	2982	2983	rBV	301	128	0.01%	0.001%
84	10.699	3002	3004	3006	rVB	280	96	0.01%	0.001%
85	10.770	3024	3026	3028	rBV2	258	121	0.01%	0.001%
86	10.924	3065	3074	3082	rVB6	2300	3602	0.31%	0.042%
87	11.143	3136	3142	3143	rBV3	924	844	0.07%	0.010%
88	11.188	3152	3156	3159	rBV2	1019	843	0.07%	0.010%
89	11.252	3165	3176	3195	rBV	474299	738883	64.34%	8.528%
90	11.426	3225	3230	3231	rBV3	954	743	0.06%	0.009%
91	11.538	3263	3265	3267	rBV2	295	163	0.01%	0.002%
92	11.625	3280	3292	3320	rBV	482343	782972	68.18%	9.037%
93	12.066	3426	3429	3431	rBV	406	281	0.02%	0.003%
94	12.426	3539	3541	3543	rBV	411	183	0.02%	0.002%
95	12.451	3547	3549	3552	rBV	349	222	0.02%	0.003%
96	12.484	3557	3559	3561	rBV	350	149	0.01%	0.002%
97	12.599	3592	3595	3596	rBV	537	262	0.02%	0.003%
98	12.622	3600	3602	3604	rBV	205	91	0.01%	0.001%
99	12.940	3699	3701	3704	rBV	317	205	0.02%	0.002%
100	13.062	3738	3739	3743	rBV2	228	162	0.01%	0.002%


Sum of corrected areas: 8664005

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091621\
Data File : VV022163.D
Acq On : 16 Sep 2021 18:09
Operator : SY/MD
Sample : M3764-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

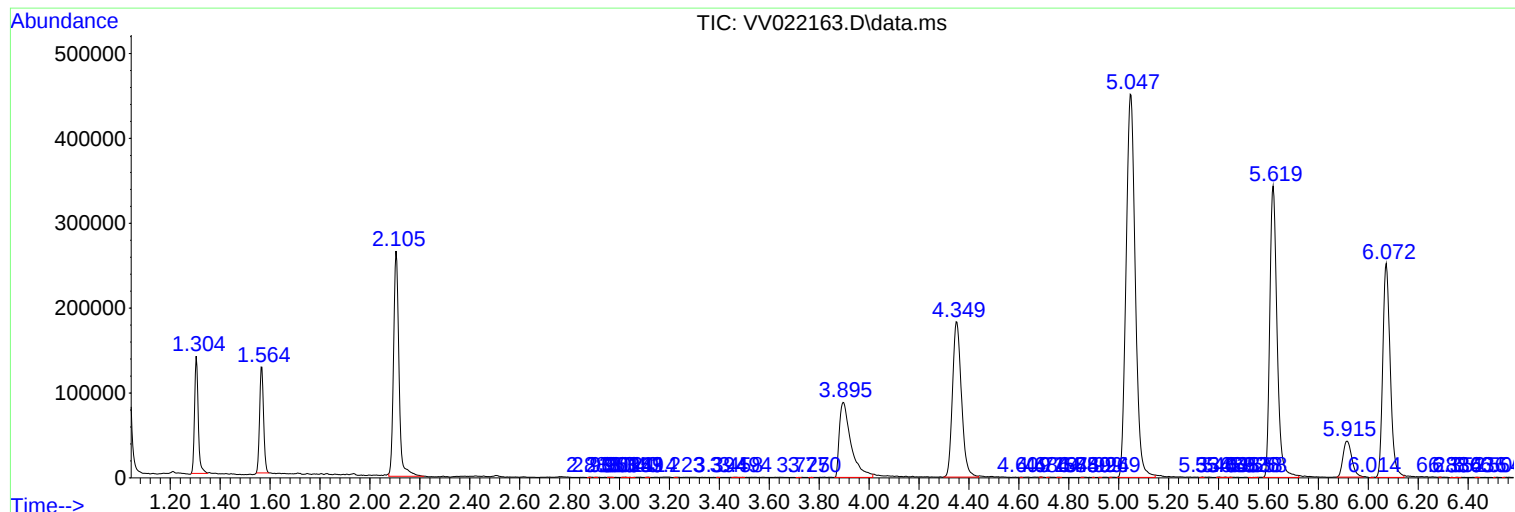

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091621\
Data File : VV022163.D
Acq On : 16 Sep 2021 18:09
Operator : SY/MD
Sample : M3764-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091621\
Data File : VV022163.D
Acq On : 16 Sep 2021 18:09
Operator : SY/MD
Sample : M3764-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
