


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091621\
 Data File : VV022149.D
 Acq On : 16 Sep 2021 08:43
 Operator : SY/MD
 Sample : BFB231
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB231

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis
 Last Update : Sat Sep 18 04:25:40 2021

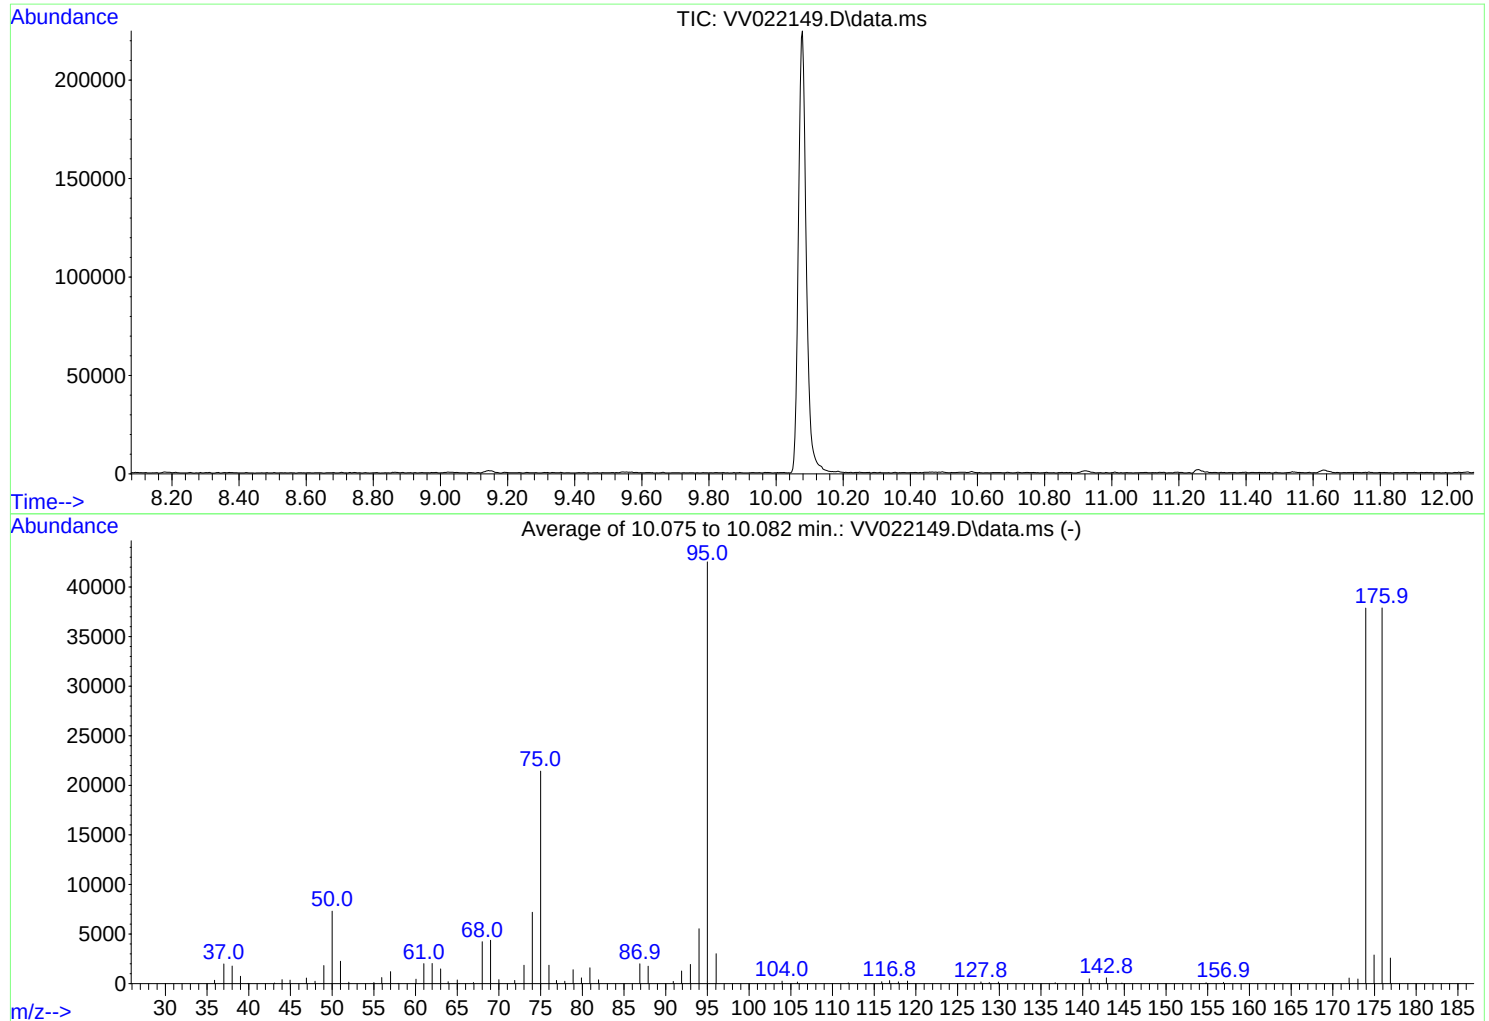

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	7316	PASS
75	95	30	80	50.4	21427	PASS
95	95	100	100	100.0	42539	PASS
96	95	5	9	7.1	3011	PASS
173	174	0.00	2	1.2	470	PASS
174	95	50	120	89.0	37872	PASS
175	174	5	9	7.6	2889	PASS
176	174	95	105	100.1	37896	PASS
177	176	5	10	6.8	2590	PASS

m/z	Abundance
35.90	347.0
37.00	2039.0
38.00	1842.0
39.00	778.0
39.90	246.0
43.10	100.0
44.00	738.0
45.00	369.0
46.90	597.0
47.90	232.0
49.00	1924.0
50.00	7519.0
51.00	2288.0
52.00	130.0
55.00	112.0
55.90	638.0
57.00	1227.0
57.90	106.0
60.00	486.0
61.00	2051.0
62.00	2098.0
63.00	1534.0
63.90	198.0
65.00	387.0
66.90	113.0
68.00	4388.0
69.00	4509.0
70.00	424.0
71.90	342.0
73.00	1942.0
74.00	7335.0
75.00	22224.0
76.00	1924.0
76.90	340.0
77.90	247.0
78.90	1428.0
79.90	597.0
80.90	1648.0
82.00	392.0
86.90	2067.0
87.90	1790.0
90.90	254.0
91.90	1333.0
93.00	1968.0
94.00	5798.0
95.00	43984.0
96.00	3056.0
104.00	276.0
105.80	166.0
111.90	106.0
115.90	210.0
116.80	327.0
117.90	193.0
119.00	250.0
127.80	183.0
128.80	122.0
129.90	177.0
136.70	136.0
140.80	495.0
142.80	613.0
144.70	104.0
154.80	121.0
156.90	129.0
171.90	592.0
173.00	484.0
174.00	39160.0
175.00	2951.0
175.90	39392.0
176.90	2684.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

Scan 2799 (10.040 min): VV022149.D\data.ms
BFB231

m/z	Abundance
40.00	207.0
44.00	295.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

m/z	Abundance
35.90	302.0
37.00	2023.0
38.00	1876.0
39.00	789.0
39.90	257.0
43.10	101.0
44.00	646.0
44.90	382.0
46.90	532.0
48.00	250.0
49.00	1810.0
50.00	7522.0
51.00	2382.0
52.00	146.0
55.00	125.0
56.00	606.0
57.00	1269.0
60.10	434.0
61.00	2179.0
62.00	2190.0
63.00	1505.0
63.90	199.0
65.00	383.0
66.90	120.0
68.00	4376.0
69.00	4638.0
70.00	395.0
71.90	329.0
73.00	1854.0
74.00	7465.0
75.00	21944.0
76.00	1854.0
76.90	325.0
77.90	251.0
78.90	1416.0
79.90	593.0
80.90	1602.0
82.00	425.0
86.90	2074.0
87.90	2003.0
90.90	252.0
91.90	1200.0
92.90	2122.0
94.00	5631.0
95.00	43832.0
96.10	3333.0
103.90	232.0
105.80	169.0
115.90	181.0
116.80	279.0
117.90	152.0
119.00	253.0
127.90	181.0
128.80	135.0
129.90	144.0
136.70	144.0
140.80	531.0
142.80	535.0
144.70	105.0
154.80	164.0
156.90	132.0
172.00	623.0
173.00	494.0
173.90	37736.0
174.90	2890.0
175.90	37976.0
176.90	2580.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

m/z	Abundance
35.90	373.0
37.00	1915.0
38.00	1615.0
39.00	687.0
39.90	219.0
44.00	712.0
45.00	324.0
46.90	582.0
47.90	229.0
49.00	1746.0
50.00	6908.0
51.00	2114.0
52.00	140.0
55.00	114.0
56.00	620.0
57.00	1143.0
60.00	462.0
61.00	1814.0
62.00	1804.0
63.00	1405.0
63.90	172.0
65.00	350.0
67.00	116.0
68.00	3903.0
69.00	3970.0
70.00	387.0
71.90	290.0
73.00	1784.0
74.00	6796.0
75.00	20112.0
76.00	1786.0
76.90	285.0
77.90	223.0
78.90	1374.0
79.90	560.0
80.90	1534.0
81.90	340.0
86.90	1845.0
87.90	1477.0
90.90	198.0
91.90	1271.0
93.00	1710.0
94.00	5169.0
95.00	39800.0
96.00	2645.0
104.00	268.0
105.80	165.0
111.90	116.0
115.90	196.0
116.90	302.0
117.90	209.0
119.00	254.0
127.70	151.0
128.80	105.0
129.90	163.0
140.80	426.0
141.80	125.0
142.90	601.0
156.90	134.0
172.00	473.0
173.00	432.0
174.00	36720.0
175.00	2827.0
175.90	36320.0
176.90	2507.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231