

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
 Data File : VV027872.D
 Acq On : 16 Sep 2022 11:08
 Operator : SY/MD
 Sample : VV0916WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK230

Quant Time: Sep 16 22:06:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 16 22:04:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	131676	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	129239	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	61471	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	36861	4.247	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	85.000%	
7) Chloroethane-d5	1.565	69	38888	5.282	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	105.600%	
11) 1,1-Dichloroethene-d2	2.105	63	62154	3.375	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.400%	
20) 2-Butanone-d5	3.912	46	67895	35.296	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	70.600%	
24) Chloroform-d	4.346	84	94627	5.324	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	106.400%	
26) 1,2-Dichloroethane-d4	5.031	65	50076	5.291	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.800%	
32) Benzene-d6	5.047	84	169795	4.529	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.600%	
36) 1,2-Dichloropropane-d6	6.066	67	46672	4.252	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	85.000%	
41) Toluene-d8	7.314	98	137768	4.370	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	87.400%	
43) trans-1,3-Dichloroprop...	7.625	79	13555	3.681	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	73.600%	
46) 2-Hexanone-d5	8.092	63	52906	38.648	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	77.300%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31343	4.446	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	89.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	50810	5.032	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	100.600%	
Target Compounds						Qvalue
16) Methylene chloride	2.507	84	10288	0.915	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027872.D
Acq On : 16 Sep 2022 11:08
Operator : SY/MD
Sample : VV0916WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK230


Quant Time: Sep 16 22:06:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 16 22:04:36 2022
Response via : Initial Calibration

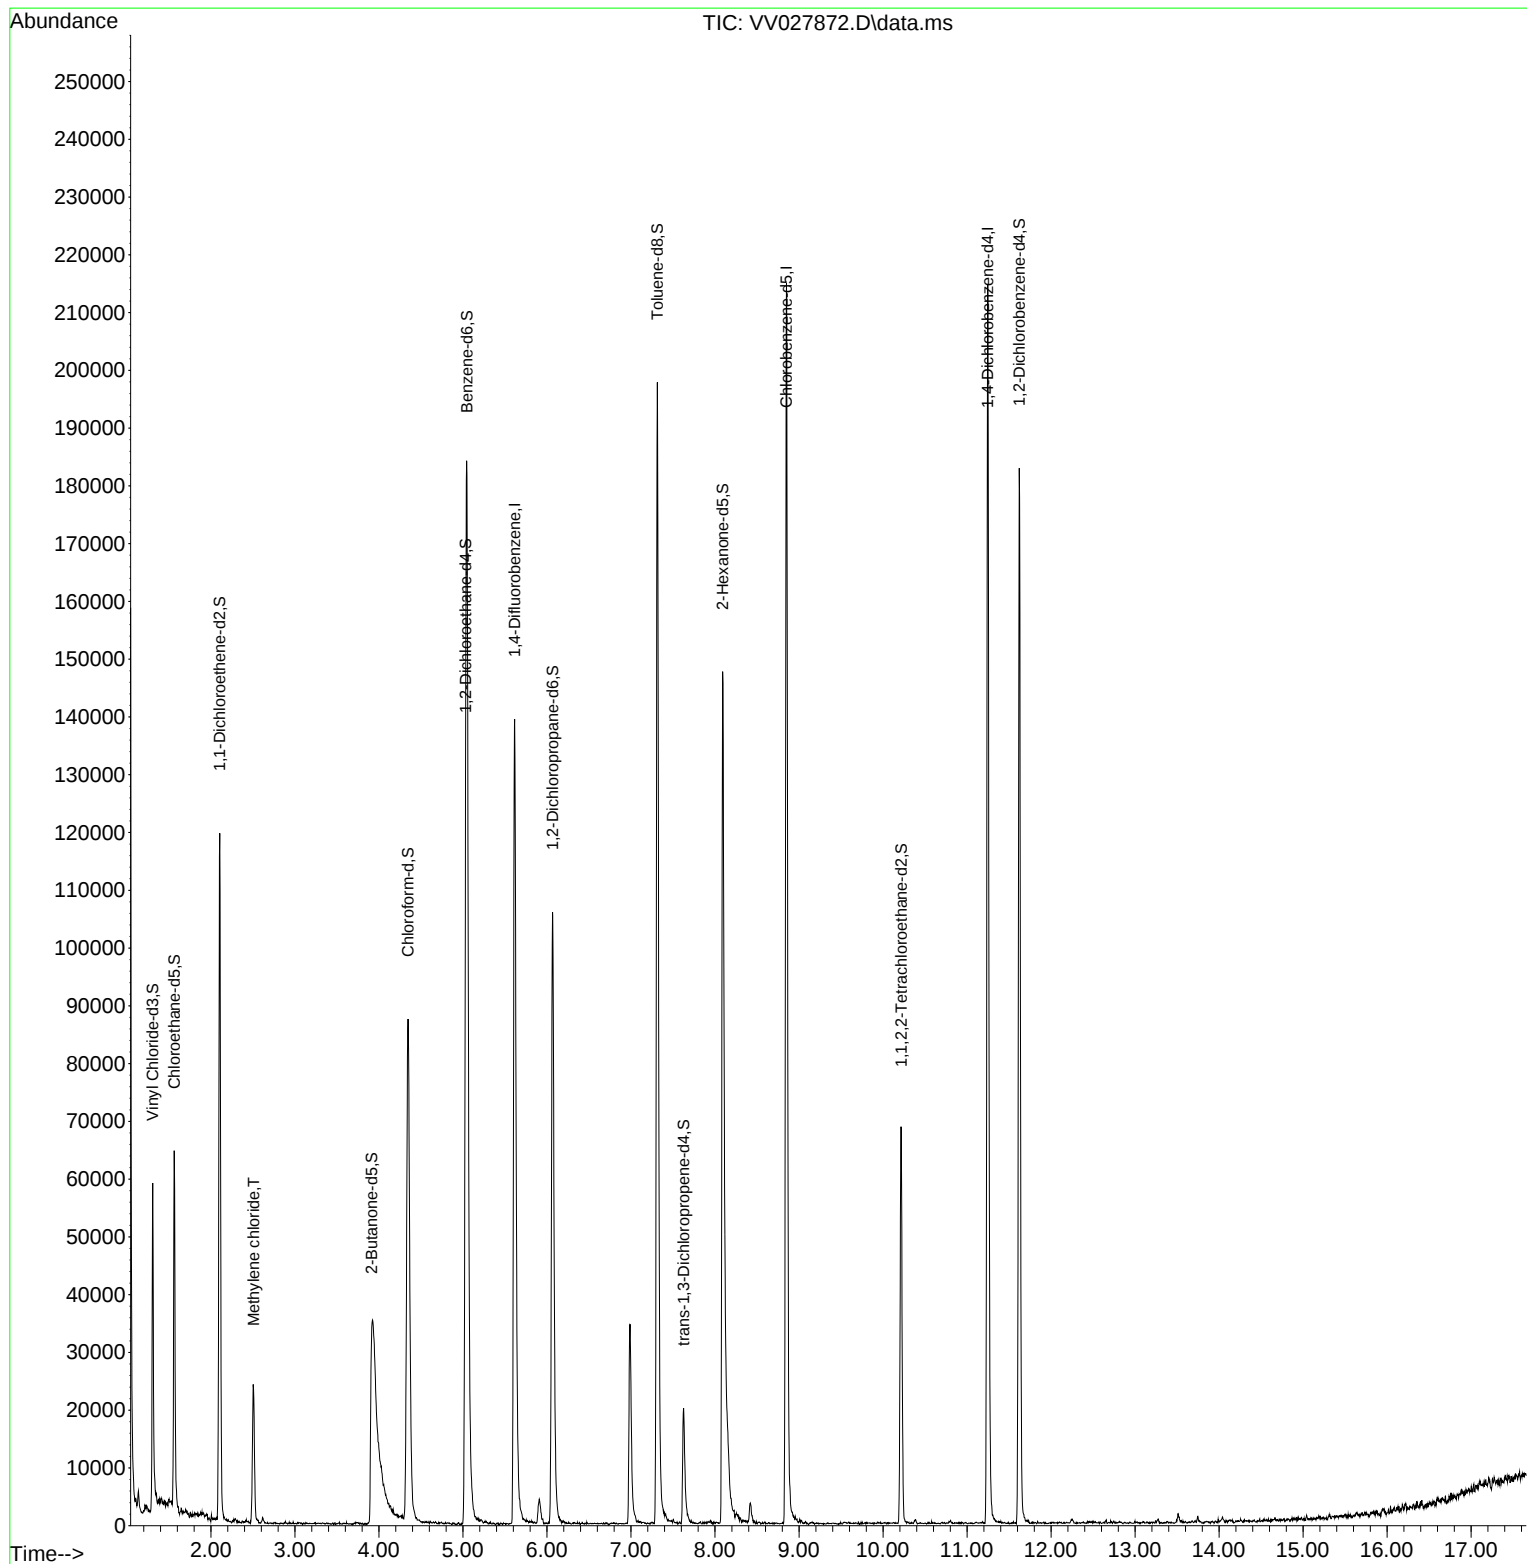

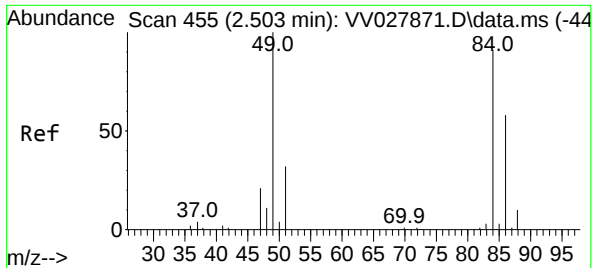

#16
Methylene chloride
Concen: 0.915 ug/L
RT: 2.507 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV027872.D
Acq: 16 Sep 2022 11:08

Instrument :
MSVOA_V
ClientSampleId :
VBLK230

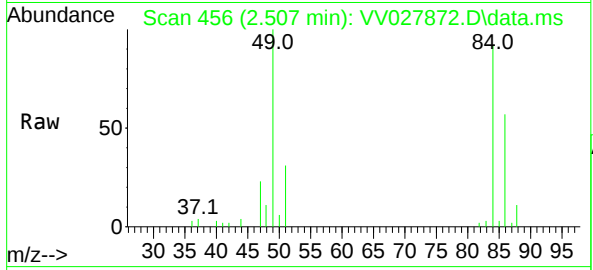

Tgt Ion: 84 Resp: 10288

Ion	Ratio	Lower	Upper
84	100		
86	62.3	44.9	83.3
49	108.3	90.1	167.3

