

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
 Data File : VV027888.D
 Acq On : 16 Sep 2022 18:03
 Operator : SY/MD
 Sample : N4658-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E81

Quant Time: Sep 16 22:10:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 16 22:04:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	133675	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	135911	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	68206	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	32067	3.639	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.800%
7) Chloroethane-d5	1.568	69	35968	4.812	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.200%
11) 1,1-Dichloroethene-d2	2.108	63	52876	2.828	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.600%#
20) 2-Butanone-d5	3.892	46	94542	48.414	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.820%
24) Chloroform-d	4.346	84	98906	5.482	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.600%
26) 1,2-Dichloroethane-d4	5.034	65	52077	5.420	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.400%
32) Benzene-d6	5.047	84	168684	4.278	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.600%
36) 1,2-Dichloropropane-d6	6.066	67	49596	4.296	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.000%
41) Toluene-d8	7.317	98	137024	4.133	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.600%
43) trans-1,3-Dichloroprop...	7.625	79	16207	4.185	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.600%
46) 2-Hexanone-d5	8.088	63	69735	48.441	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.880%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	35335	4.767	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	57597	5.141	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.800%
Target Compounds					Qvalue	
25) Chloroform	4.378	83	15191	0.780	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027888.D
Acq On : 16 Sep 2022 18:03
Operator : SY/MD
Sample : N4658-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E81

Quant Time: Sep 16 22:10:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 16 22:04:36 2022
Response via : Initial Calibration

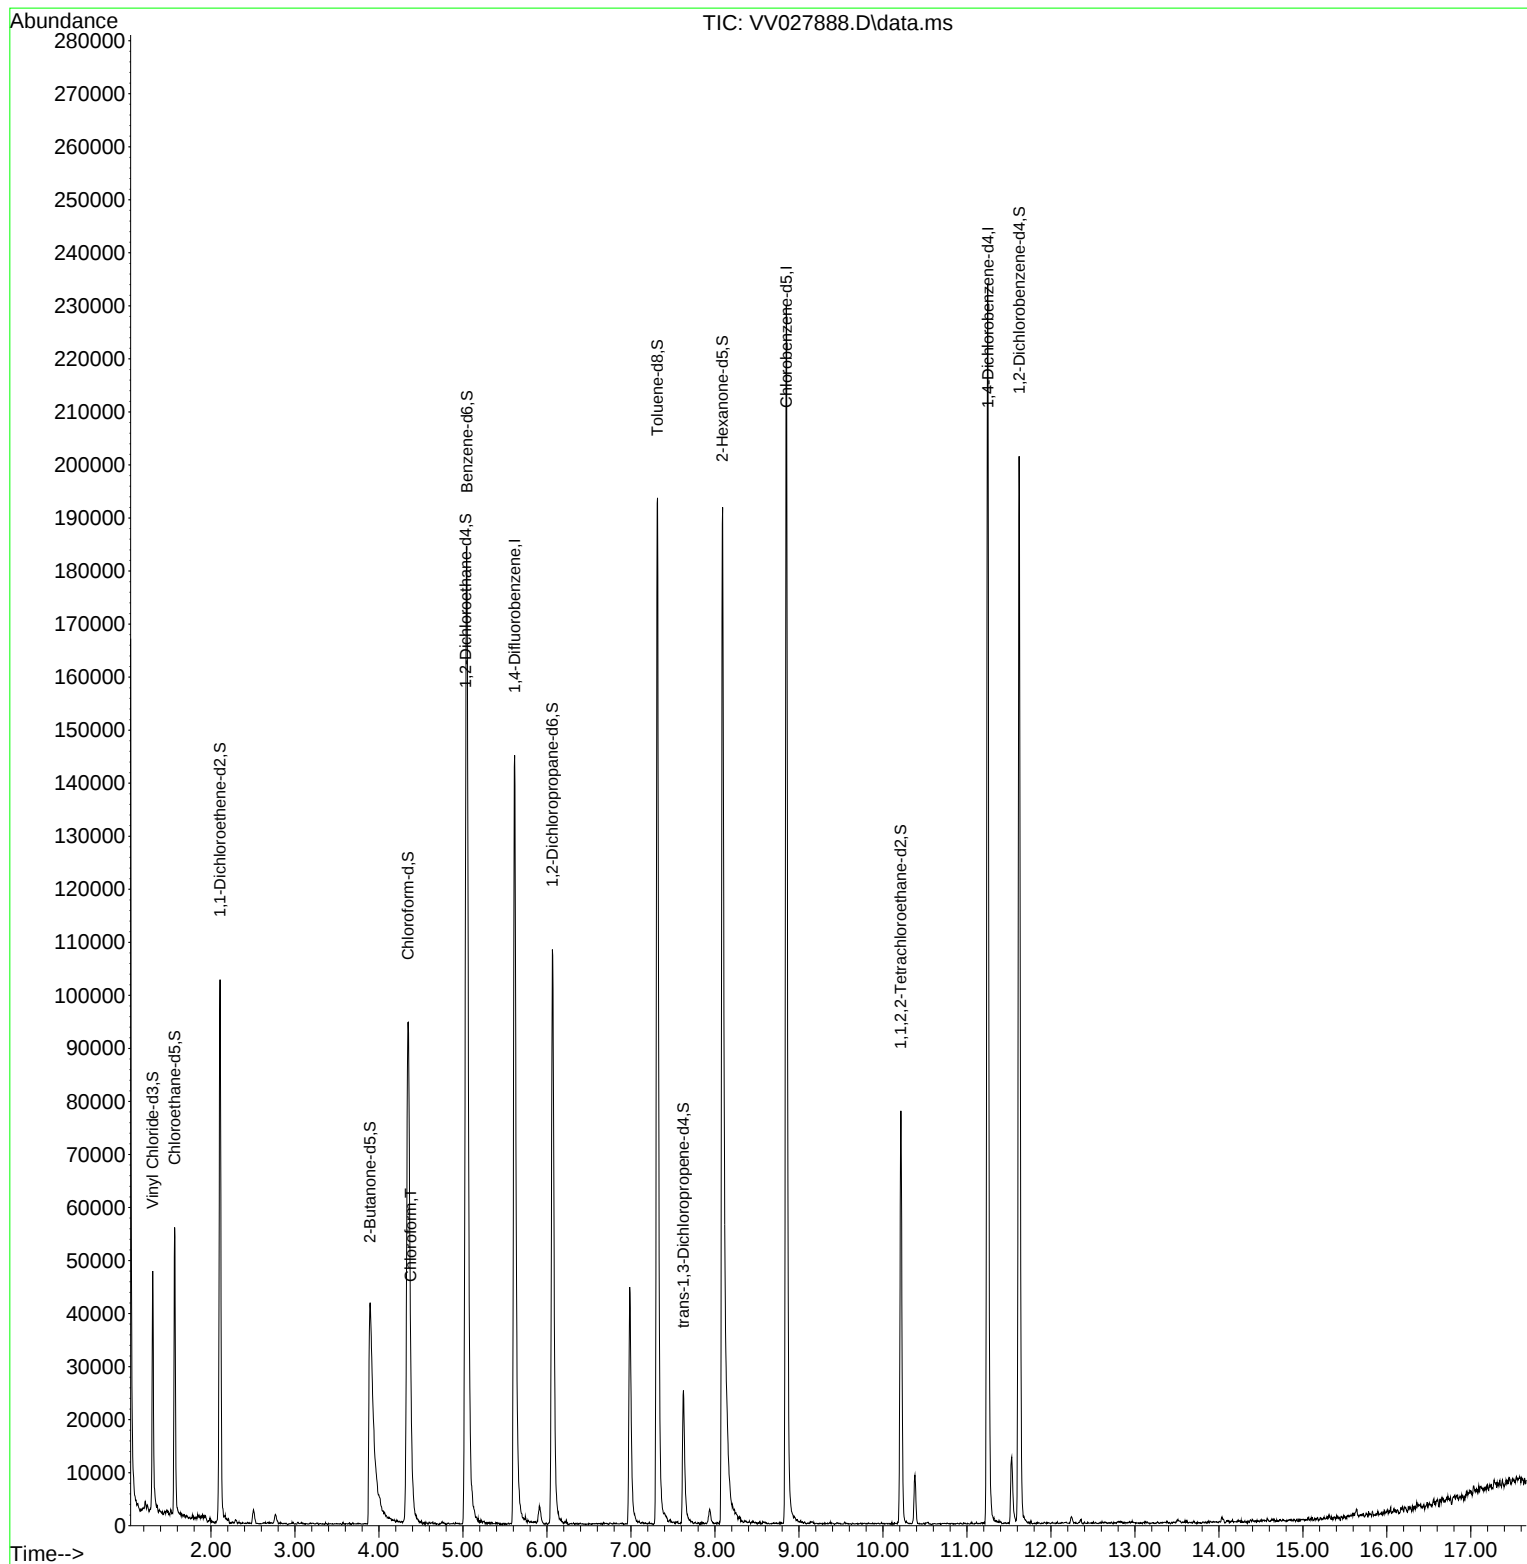

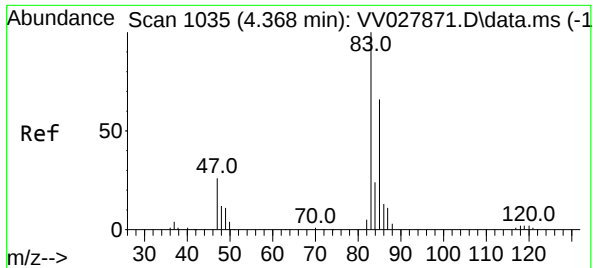

#25
 Chloroform
 Concen: 0.780 ug/L
 RT: 4.378 min Scan# 10
 Delta R.T. 0.010 min
 Lab File: VV027888.D
 Acq: 16 Sep 2022 18:03

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E81

Tgt Ion: 83 Resp: 15191
 Ion Ratio Lower Upper
 83 100
 85 65.7 45.4 84.2

