

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
 Data File : VV027872.D
 Acq On : 16 Sep 2022 11:08
 Operator : SY/MD
 Sample : VV0916WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK230

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027872.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	95	rBV	56943	65692	14.13%	1.812%
2	1.561	155	162	179	rVB	62668	78027	16.79%	2.152%
3	2.105	321	331	345	rBV	118865	171140	36.82%	4.720%
4	2.503	445	455	467	rBV3	24006	39048	8.40%	1.077%
5	3.925	881	897	918	rBV3	35172	151111	32.51%	4.168%
6	4.346	1012	1028	1057	rBV3	86529	223779	48.15%	6.172%
7	5.044	1229	1245	1276	rBV3	183994	464790	100.00%	12.820%
8	5.616	1411	1423	1454	rBV	139206	293213	63.09%	8.088%
9	5.908	1504	1514	1526	rBV5	4137	8902	1.92%	0.246%
10	6.066	1550	1563	1587	rBV2	105802	220027	47.34%	6.069%
11	6.986	1839	1849	1874	rBV	34501	68635	14.77%	1.893%
12	7.314	1939	1951	1974	rBV	197571	354378	76.24%	9.775%
13	7.625	2039	2048	2062	rBV2	20049	38241	8.23%	1.055%
14	8.092	2181	2193	2231	rBV2	147394	336876	72.48%	9.292%
15	8.420	2284	2295	2305	rBV5	3418	6330	1.36%	0.175%
16	8.850	2418	2429	2450	rBV	214681	362823	78.06%	10.008%
17	10.214	2842	2853	2869	rBV2	68684	111059	23.89%	3.063%
18	11.246	3164	3174	3192	rBV	214522	340643	73.29%	9.396%
19	11.622	3280	3291	3310	rBV	182693	290789	62.56%	8.021%




Sum of corrected areas: 3625503

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027872.D
Acq On : 16 Sep 2022 11:08
Operator : SY/MD
Sample : VV0916WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK230

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

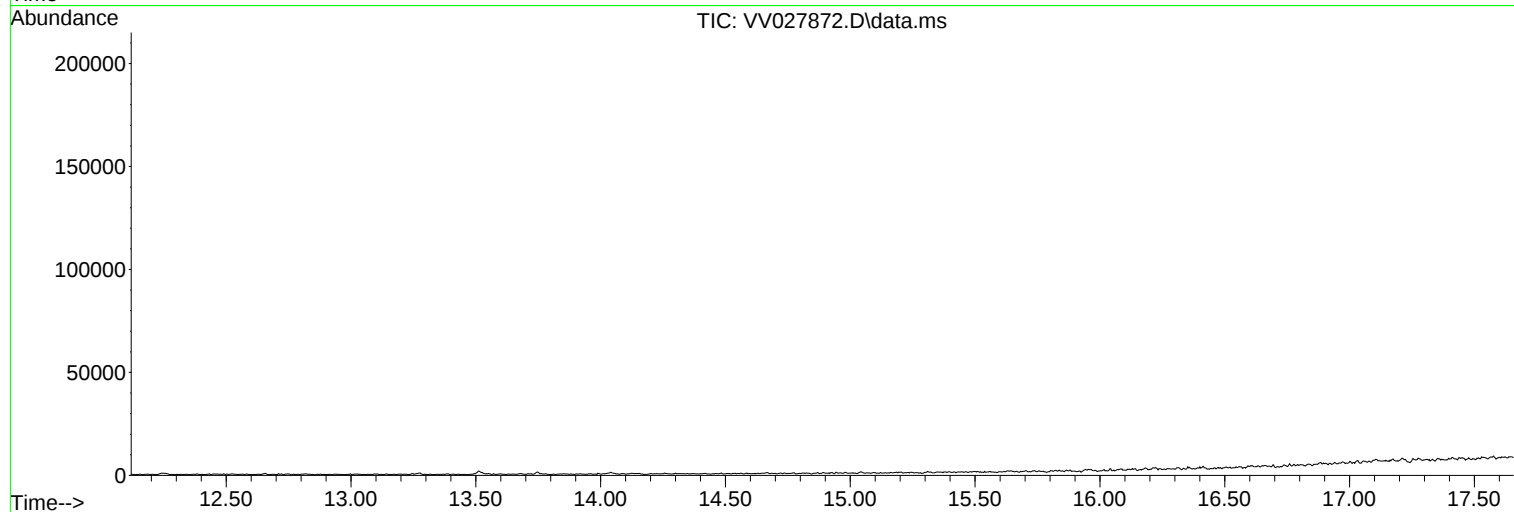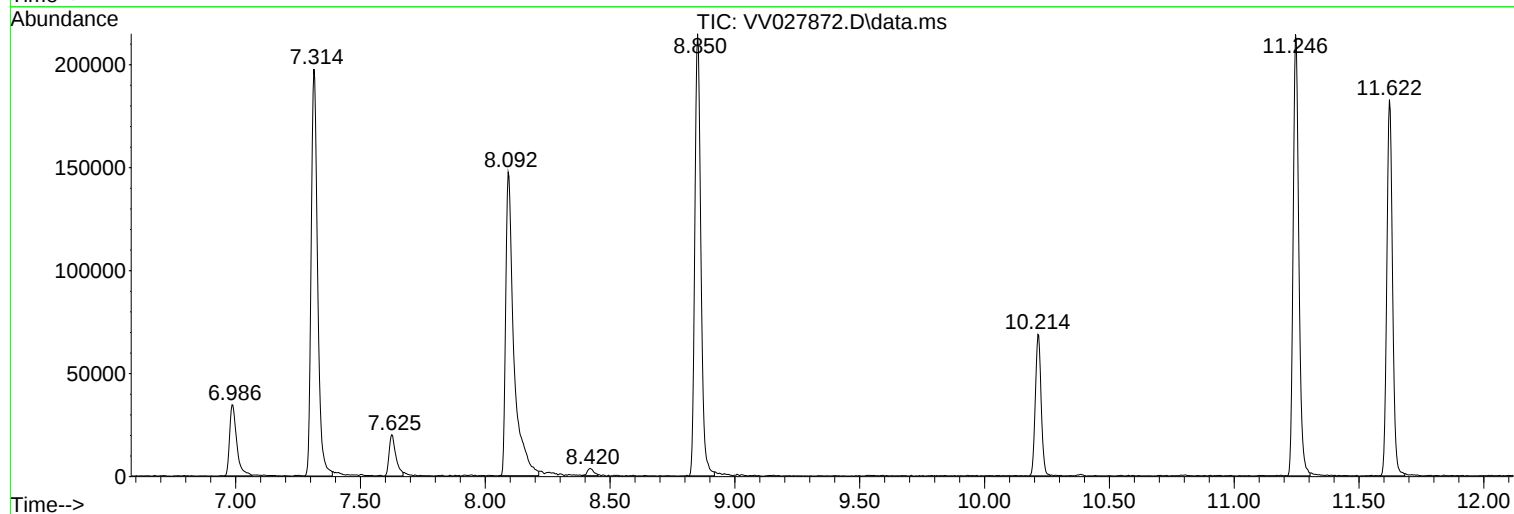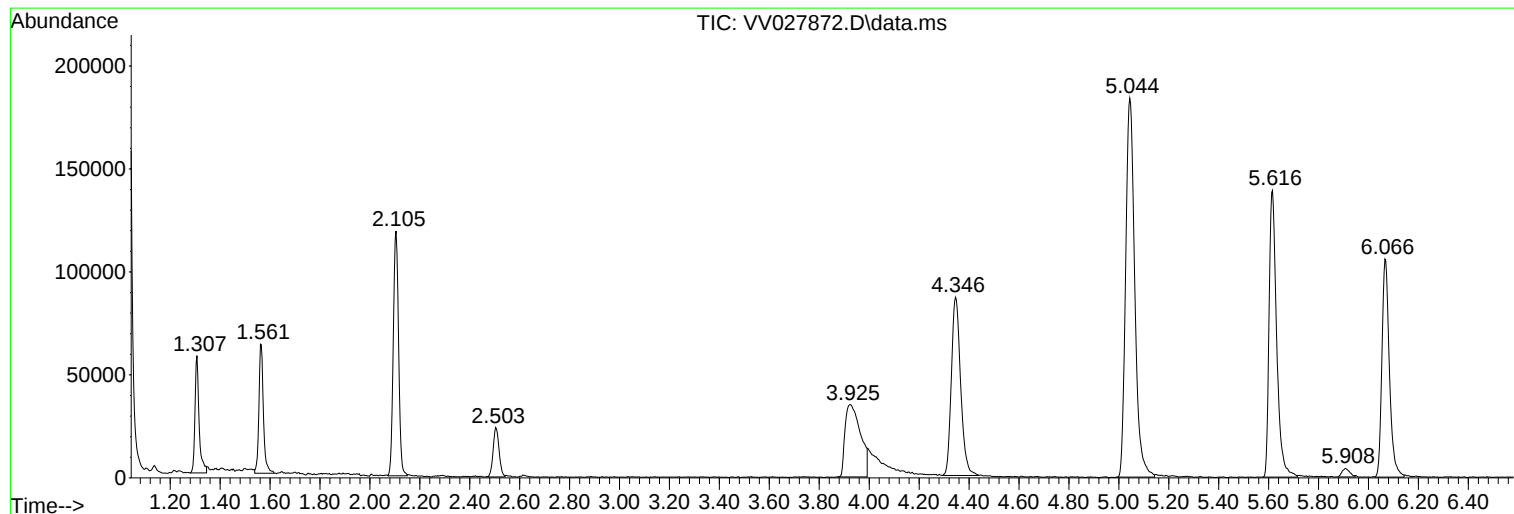

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027872.D
Acq On : 16 Sep 2022 11:08
Operator : SY/MD
Sample : VV0916WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK230

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027872.D
Acq On : 16 Sep 2022 11:08
Operator : SY/MD
Sample : VV0916WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK230

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc