

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
 Data File : VV027873.D
 Acq On : 16 Sep 2022 11:36
 Operator : SY/MD
 Sample : N4652-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ23

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027873.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rBV	41348	48970	5.26%	1.071%
2	1.568	156	164	177	rVB	50775	59732	6.41%	1.307%
3	2.104	320	331	351	rBB2	101696	151922	16.31%	3.324%
4	2.764	525	536	552	rVB9	6006	13277	1.43%	0.290%
5	3.185	653	667	683	rBV	53191	112991	12.13%	2.472%
6	3.908	880	892	920	rBV2	37993	130987	14.06%	2.866%
7	4.342	1009	1027	1052	rBV2	81201	207992	22.33%	4.551%
8	4.600	1087	1107	1131	rBV	371659	931648	100.00%	20.384%
9	5.043	1229	1245	1273	rBV3	170146	431688	46.34%	9.445%
10	5.612	1409	1422	1447	rBV	152600	315349	33.85%	6.900%
11	5.915	1503	1516	1537	rBV6	19076	45673	4.90%	0.999%
12	6.066	1548	1563	1583	rBV	98878	208428	22.37%	4.560%
13	6.985	1840	1849	1865	rBV2	35177	68429	7.34%	1.497%
14	7.313	1940	1951	1974	rBV	178182	324438	34.82%	7.098%
15	7.625	2037	2048	2066	rBV2	21067	39580	4.25%	0.866%
16	7.937	2133	2145	2156	rBV2	9293	16376	1.76%	0.358%
17	8.091	2182	2193	2236	rBV2	115978	313430	33.64%	6.858%
18	8.850	2417	2429	2452	rBV	230739	384894	41.31%	8.421%
19	10.213	2843	2853	2871	rBV2	59788	98694	10.59%	2.159%
20	10.381	2895	2905	2915	rBV	16453	26697	2.87%	0.584%
21	11.246	3163	3174	3194	rBV	222768	355212	38.13%	7.772%
22	11.622	3278	3291	3306	rBV	175112	274480	29.46%	6.005%
23	15.969	4631	4643	4646	rBV	5192	9660	1.04%	0.211%




Sum of corrected areas: 4570547

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027873.D
Acq On : 16 Sep 2022 11:36
Operator : SY/MD
Sample : N4652-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

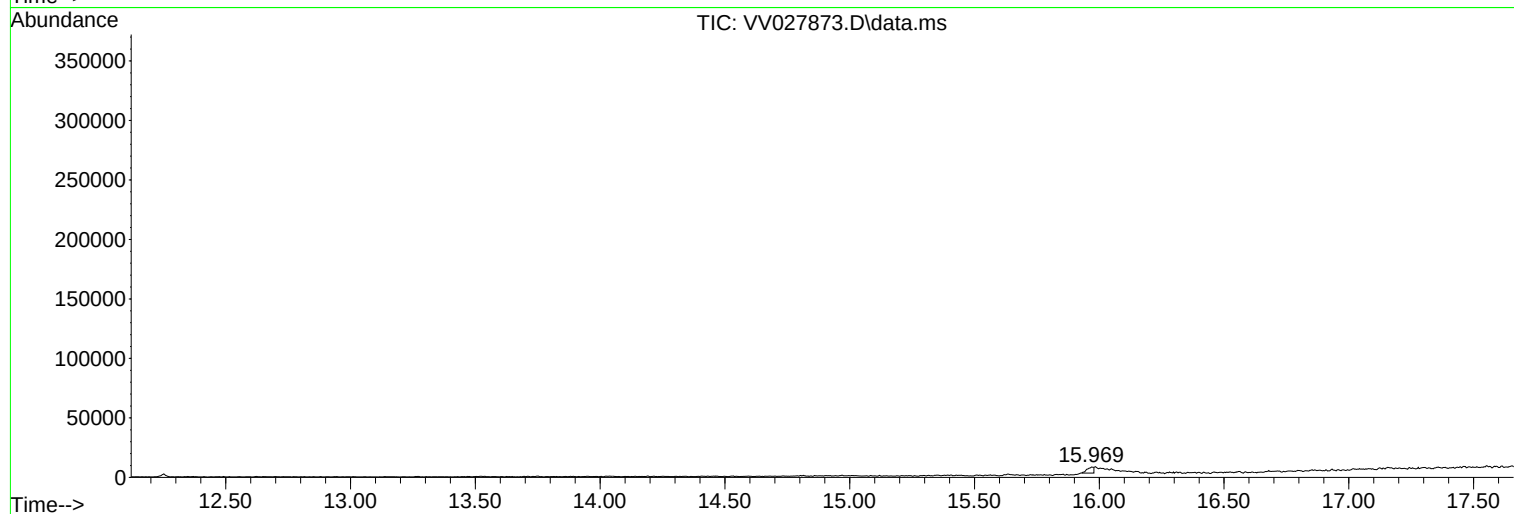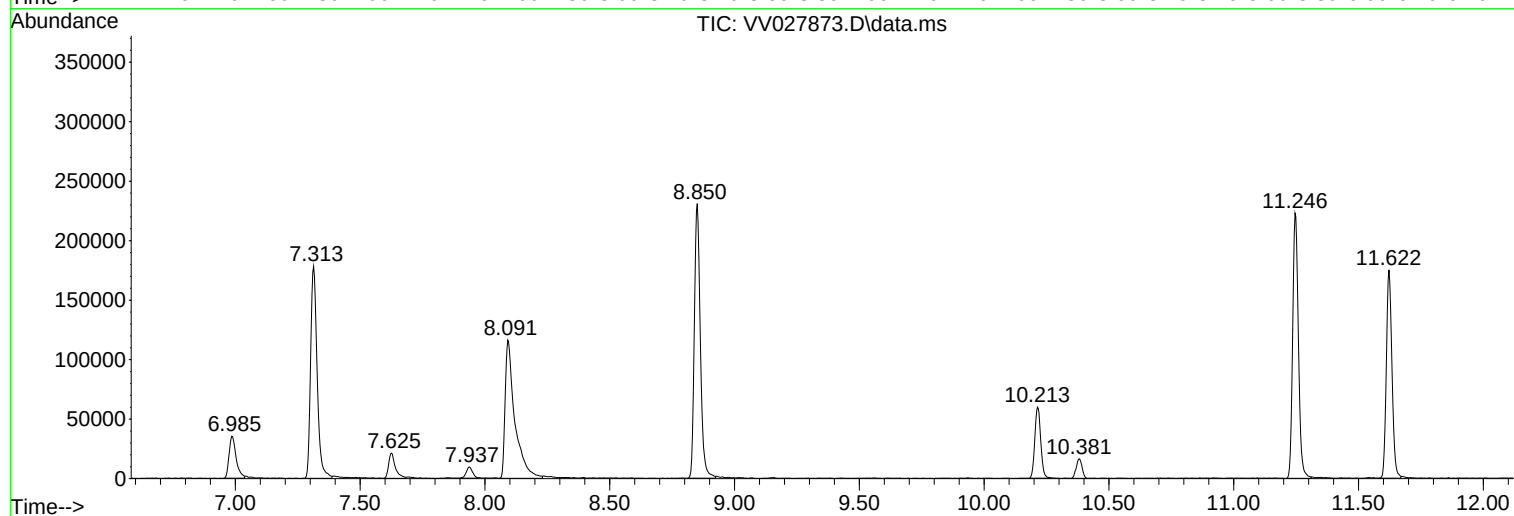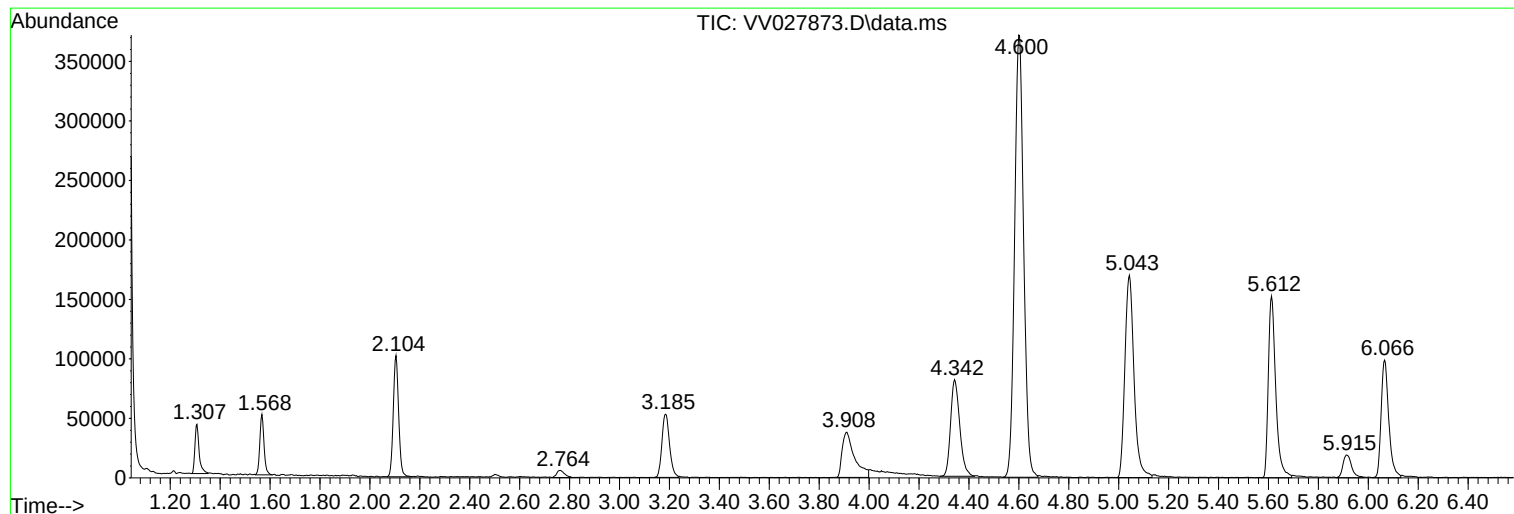

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027873.D
Acq On : 16 Sep 2022 11:36
Operator : SY/MD
Sample : N4652-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027873.D
Acq On : 16 Sep 2022 11:36
Operator : SY/MD
Sample : N4652-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------