

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
 Data File : VV027874.D
 Acq On : 16 Sep 2022 12:00
 Operator : SY/MD
 Sample : N4652-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ24

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027874.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	97	rBV	42086	49878	11.76%	1.452%
2	1.568	156	164	181	rBV	53831	65067	15.35%	1.895%
3	2.105	322	331	345	rBV	83631	121503	28.66%	3.538%
4	2.507	446	456	466	rVB7	3180	5545	1.31%	0.161%
5	3.191	656	669	681	rBV2	4106	8015	1.89%	0.233%
6	3.896	873	888	919	rBV2	35031	129998	30.66%	3.785%
7	4.346	1011	1028	1053	rBV2	83506	211677	49.93%	6.163%
8	5.043	1230	1245	1273	rBV2	167944	423974	100.00%	12.345%
9	5.616	1411	1423	1446	rBV	140737	296689	69.98%	8.639%
10	6.066	1546	1563	1586	rBV2	98664	206222	48.64%	6.004%
11	6.989	1839	1850	1877	rBV	35803	70704	16.68%	2.059%
12	7.313	1940	1951	1972	rBV	177451	316361	74.62%	9.211%
13	7.625	2037	2048	2069	rBV3	20543	39119	9.23%	1.139%
14	7.937	2135	2145	2158	rBV2	11195	19691	4.64%	0.573%
15	8.092	2180	2193	2225	rBV2	141934	326129	76.92%	9.496%
16	8.850	2418	2429	2457	rBV	224912	377867	89.13%	11.002%
17	10.214	2842	2853	2869	rBV2	65062	102692	24.22%	2.990%
18	10.381	2895	2905	2918	rBV2	25387	40006	9.44%	1.165%
19	11.246	3163	3174	3194	rBV	215826	341222	80.48%	9.935%
20	11.622	3279	3291	3313	rBV	170887	275635	65.01%	8.026%
21	12.252	3476	3487	3496	rVB2	4179	6483	1.53%	0.189%




Sum of corrected areas: 3434477

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027874.D
Acq On : 16 Sep 2022 12:00
Operator : SY/MD
Sample : N4652-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

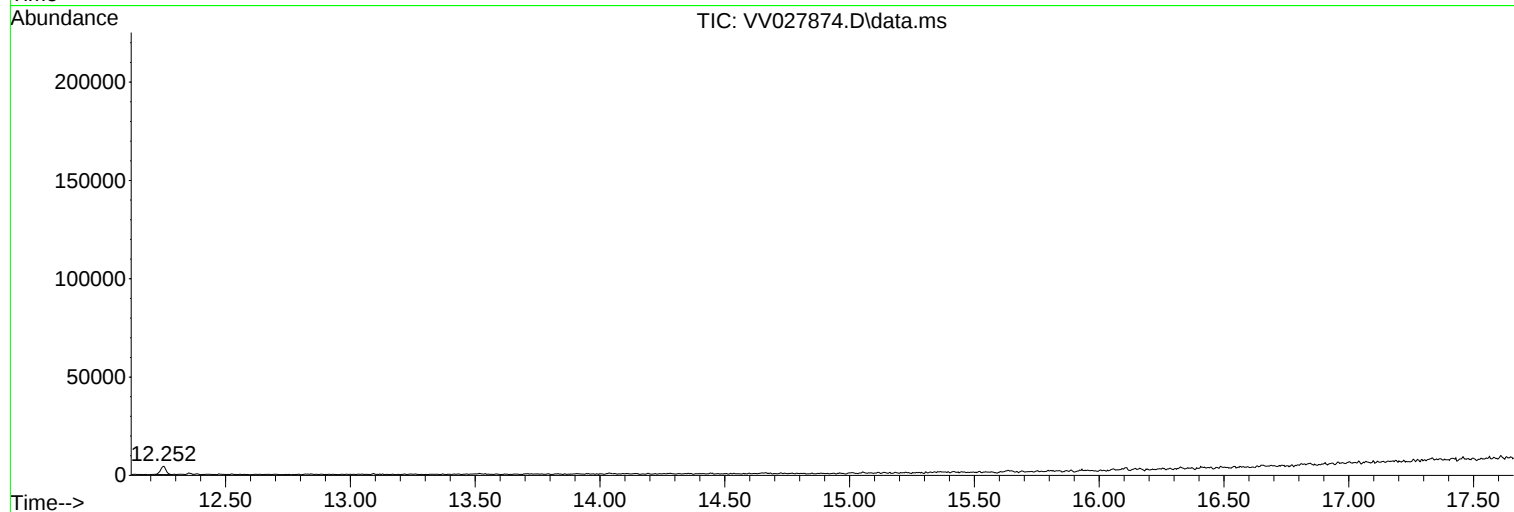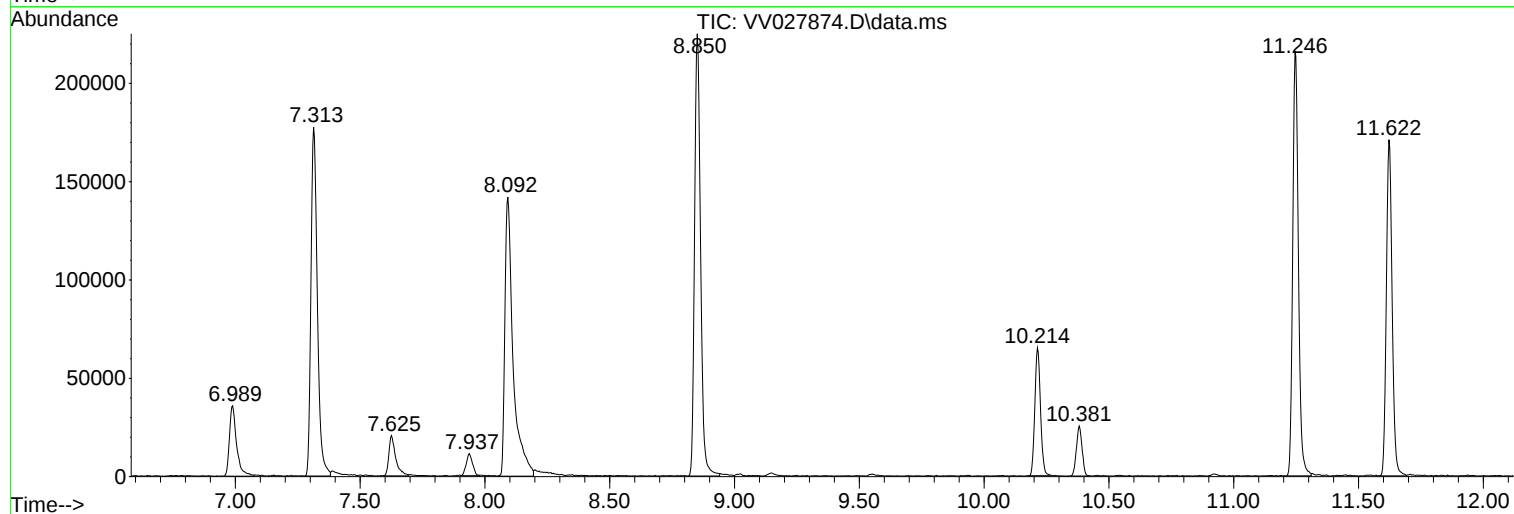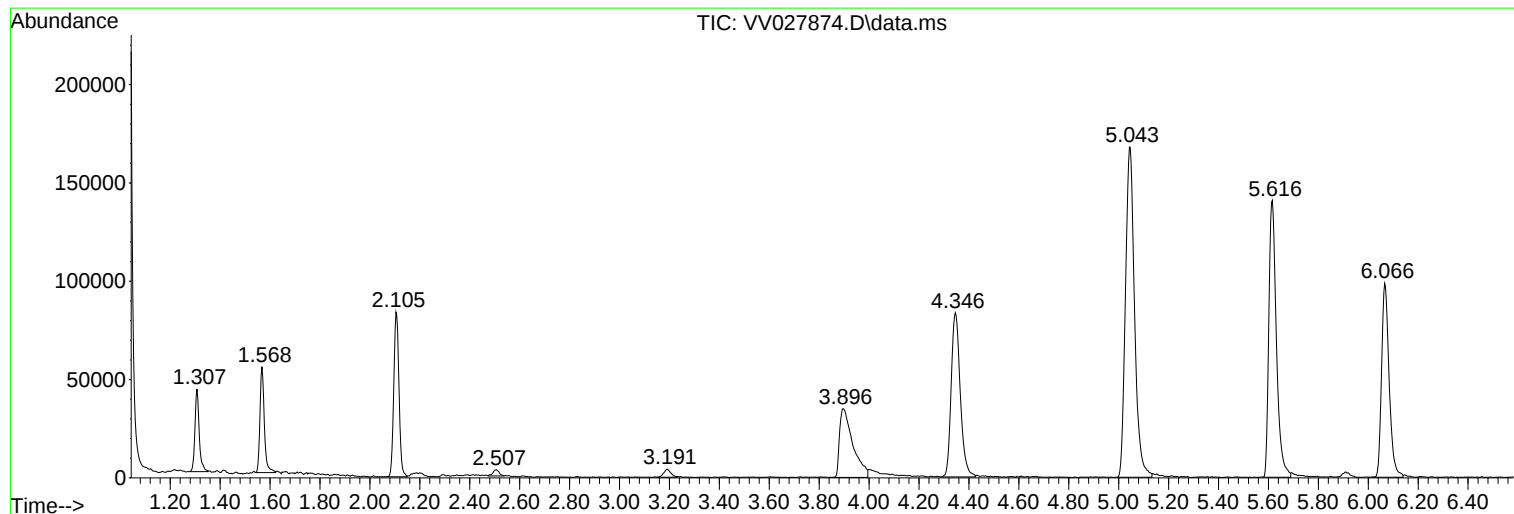

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027874.D
Acq On : 16 Sep 2022 12:00
Operator : SY/MD
Sample : N4652-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027874.D
Acq On : 16 Sep 2022 12:00
Operator : SY/MD
Sample : N4652-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------