

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
 Data File : VV027875.D
 Acq On : 16 Sep 2022 12:24
 Operator : SY/MD
 Sample : N4652-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ27

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027875.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	98	rBV	47662	54240	12.57%	1.437%
2	1.568	157	164	178	rVB	53993	64387	14.92%	1.706%
3	2.105	319	331	346	rBV	97883	148614	34.45%	3.937%
4	2.503	449	455	467	rVB6	4900	7756	1.80%	0.205%
5	2.767	527	537	553	rBV5	7276	15064	3.49%	0.399%
6	3.188	655	668	689	rBV2	22035	46734	10.83%	1.238%
7	3.908	879	892	931	rBV2	79018	255493	59.22%	6.768%
8	4.349	1012	1029	1053	rBV	83739	213609	49.51%	5.658%
9	4.603	1094	1108	1109	rBV	4769	5293	1.23%	0.140%
10	5.043	1230	1245	1267	rBV3	173443	431443	100.00%	11.429%
11	5.616	1411	1423	1453	rBV	144579	302320	70.07%	8.008%
12	5.921	1503	1518	1538	rVB7	11429	27046	6.27%	0.716%
13	6.066	1550	1563	1584	rBV2	100632	209151	48.48%	5.540%
14	6.989	1839	1850	1866	rBV2	35536	70467	16.33%	1.867%
15	7.313	1940	1951	1971	rBV	183805	332023	76.96%	8.795%
16	7.625	2039	2048	2068	rBV	22572	41114	9.53%	1.089%
17	7.934	2133	2144	2150	rBV2	7088	12480	2.89%	0.331%
18	7.976	2152	2157	2170	rVB4	9839	15828	3.67%	0.419%
19	8.092	2181	2193	2226	rBV2	152714	339538	78.70%	8.994%
20	8.850	2417	2429	2459	rBV	226654	381581	88.44%	10.108%
21	10.214	2842	2853	2872	rBV	70416	111753	25.90%	2.960%
22	10.381	2894	2905	2917	rVB2	18308	29435	6.82%	0.780%
23	11.001	3091	3098	3107	rBV5	5518	8945	2.07%	0.237%
24	11.249	3164	3175	3197	rBV	223027	356325	82.59%	9.439%
25	11.622	3280	3291	3308	rBV2	183560	288936	66.97%	7.654%
26	12.249	3477	3486	3495	rBV3	3444	5488	1.27%	0.145%




Sum of corrected areas: 3775063

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027875.D
Acq On : 16 Sep 2022 12:24
Operator : SY/MD
Sample : N4652-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

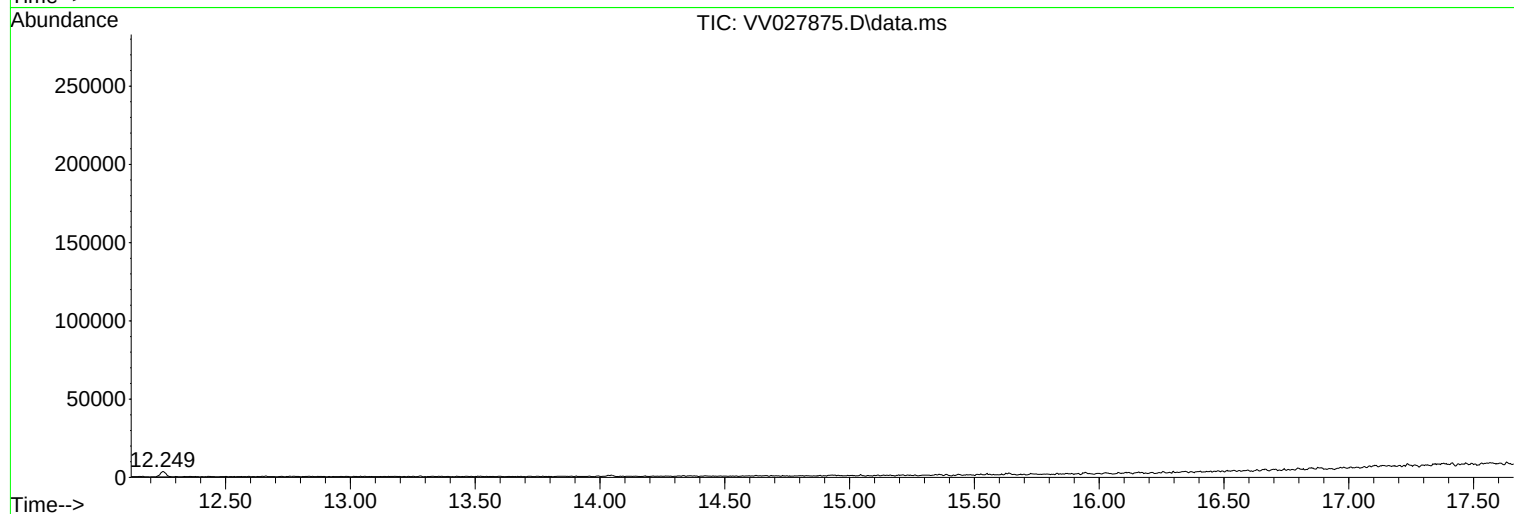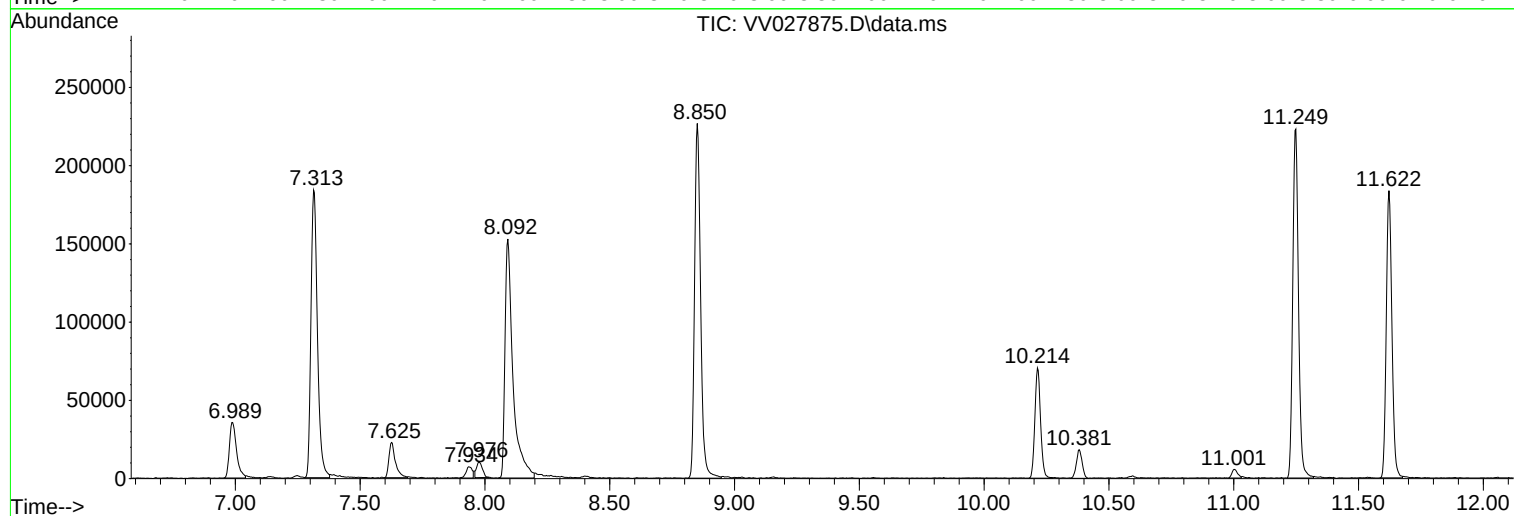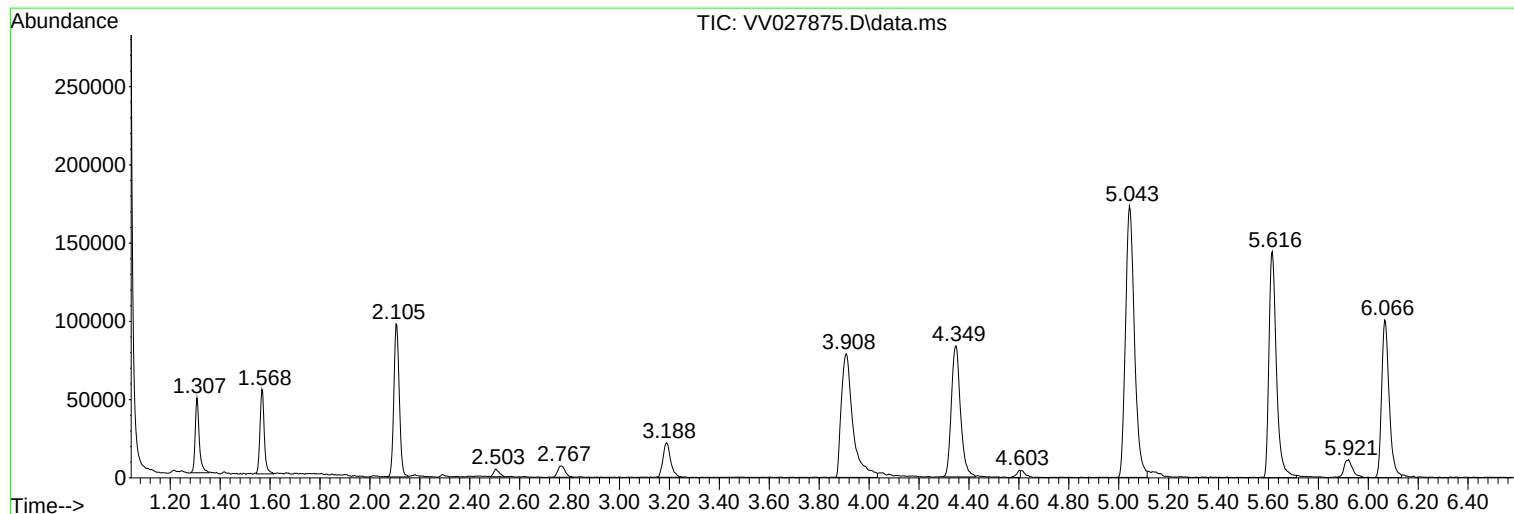

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027875.D
Acq On : 16 Sep 2022 12:24
Operator : SY/MD
Sample : N4652-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027875.D
Acq On : 16 Sep 2022 12:24
Operator : SY/MD
Sample : N4652-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc