

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
 Data File : VV027876.D
 Acq On : 16 Sep 2022 12:49
 Operator : SY/MD
 Sample : N4652-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ28

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027876.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	17	21	33	rVB2	7788	9920	2.37%	0.283%
2	1.307	74	83	99	rVB	46896	58696	14.01%	1.673%
3	1.568	157	164	178	rBV	53530	63804	15.23%	1.818%
4	2.108	321	332	348	rVB	85291	124806	29.78%	3.557%
5	2.291	382	389	397	rBV	3753	5472	1.31%	0.156%
6	3.188	655	668	682	rBV2	9144	18964	4.53%	0.540%
7	3.896	875	888	925	rBV	33954	125380	29.92%	3.573%
8	4.346	1011	1028	1054	rBV2	81862	207520	49.52%	5.914%
9	4.606	1096	1109	1123	rBV5	5461	13700	3.27%	0.390%
10	5.043	1229	1245	1269	rBV2	163638	419058	100.00%	11.943%
11	5.616	1411	1423	1446	rBV2	143135	294497	70.28%	8.393%
12	5.915	1506	1516	1517	rBV2	10480	10298	2.46%	0.293%
13	6.066	1551	1563	1588	rBV2	95669	204113	48.71%	5.817%
14	6.989	1839	1850	1867	rBV	34593	65961	15.74%	1.880%
15	7.313	1938	1951	1969	rBV	175175	316063	75.42%	9.007%
16	7.625	2036	2048	2069	rBV2	18879	37817	9.02%	1.078%
17	7.937	2133	2145	2148	rBV2	7438	10921	2.61%	0.311%
18	7.976	2151	2157	2178	rVB3	18784	31860	7.60%	0.908%
19	8.091	2183	2193	2236	rBV	144829	329293	78.58%	9.384%
20	8.850	2414	2429	2455	rBV	228290	377417	90.06%	10.756%
21	9.436	2601	2611	2619	rBV4	3079	5118	1.22%	0.146%
22	10.214	2843	2853	2870	rBV	65326	105148	25.09%	2.997%
23	10.381	2895	2905	2916	rVB	18945	30188	7.20%	0.860%
24	11.246	3164	3174	3195	rBV	213848	343965	82.08%	9.803%
25	11.622	3280	3291	3311	rBV	171392	277044	66.11%	7.895%
26	12.249	3474	3486	3498	rBV3	4470	6828	1.63%	0.195%
27	12.670	3605	3617	3630	rBV2	9717	15065	3.59%	0.429%




Sum of corrected areas: 3508916

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027876.D
Acq On : 16 Sep 2022 12:49
Operator : SY/MD
Sample : N4652-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

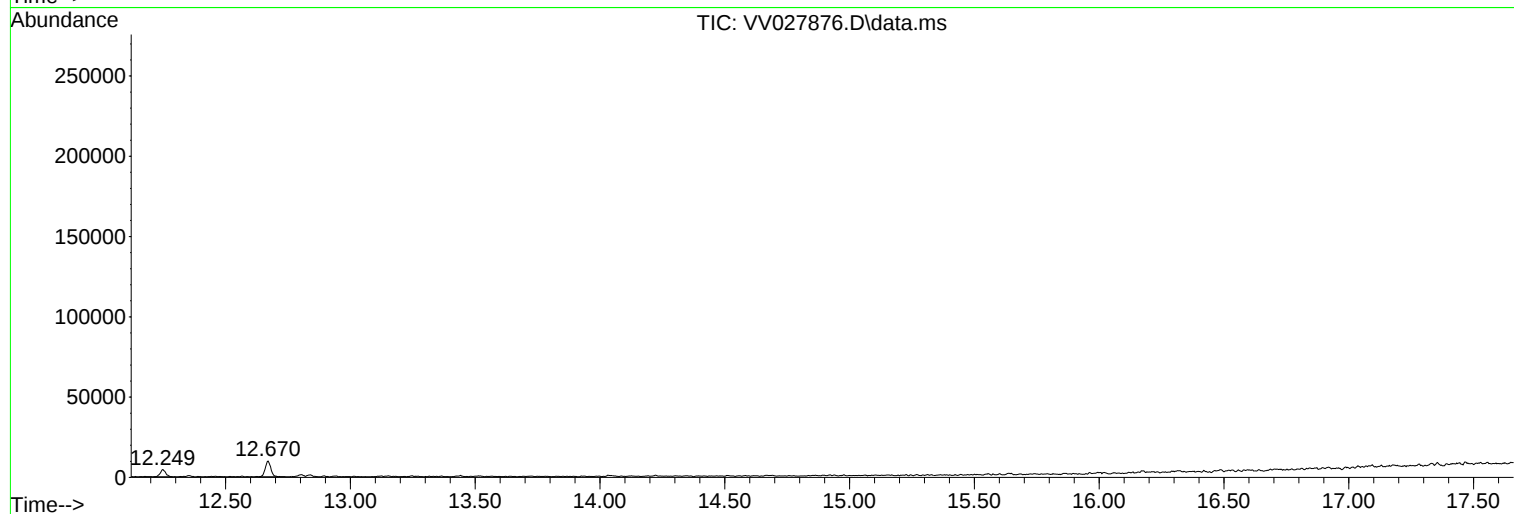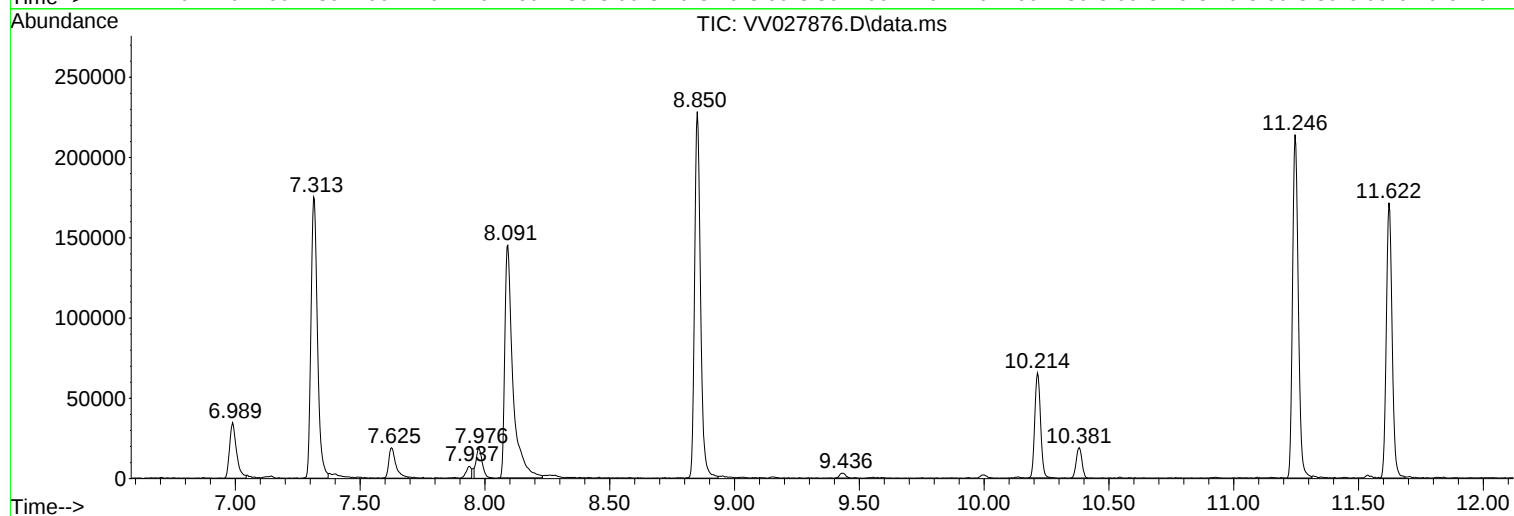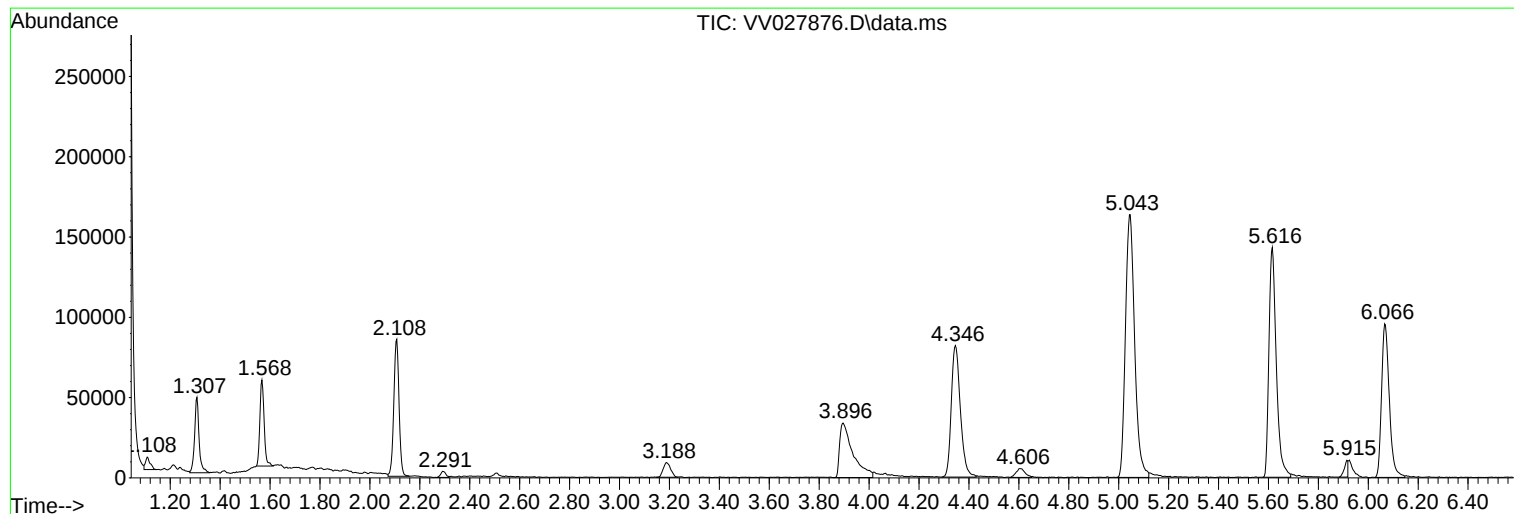

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027876.D
Acq On : 16 Sep 2022 12:49
Operator : SY/MD
Sample : N4652-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027876.D
Acq On : 16 Sep 2022 12:49
Operator : SY/MD
Sample : N4652-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc