

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
 Data File : VV027878.D
 Acq On : 16 Sep 2022 13:37
 Operator : SY/MD
 Sample : N4618-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E60

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027878.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	46	50	57	rBV3	4597	5042	1.08%	0.140%
2	1.307	73	83	96	rVV	47979	59106	12.67%	1.643%
3	1.568	157	164	180	rVB	60383	71680	15.37%	1.993%
4	2.105	320	331	346	rVB	92216	135253	29.00%	3.761%
5	3.889	878	886	923	rBV	36195	133274	28.57%	3.705%
6	4.346	1012	1028	1052	rBV	89199	227494	48.77%	6.325%
7	5.043	1229	1245	1277	rBV2	185801	466451	100.00%	12.969%
8	5.616	1411	1423	1447	rBV	145305	299261	64.16%	8.320%
9	5.915	1506	1516	1530	rVB5	2715	6228	1.34%	0.173%
10	6.066	1550	1563	1582	rBV3	105133	216696	46.46%	6.025%
11	6.989	1839	1850	1877	rBV	41199	81658	17.51%	2.270%
12	7.313	1939	1951	1973	rBV	191440	343372	73.61%	9.547%
13	7.625	2040	2048	2067	rBV2	24770	44295	9.50%	1.232%
14	8.088	2180	2192	2225	rBV	157899	355761	76.27%	9.891%
15	8.850	2418	2429	2451	rBV	229357	374278	80.24%	10.406%
16	10.214	2842	2853	2869	rBV2	72559	114871	24.63%	3.194%
17	10.384	2895	2906	2913	rBV3	4852	8192	1.76%	0.228%
18	11.249	3164	3175	3196	rBV	221463	342707	73.47%	9.528%
19	11.532	3255	3263	3274	rBV6	5177	8990	1.93%	0.250%
20	11.622	3280	3291	3310	rBV	188098	302062	64.76%	8.398%




Sum of corrected areas: 3596671

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027878.D
Acq On : 16 Sep 2022 13:37
Operator : SY/MD
Sample : N4618-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

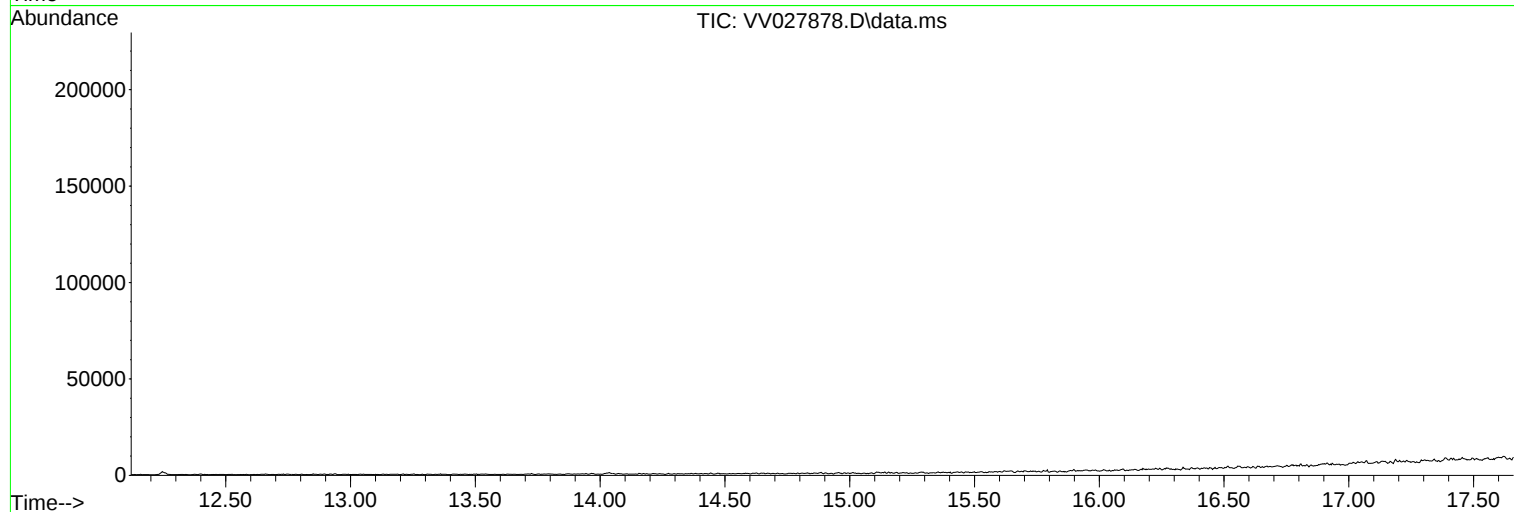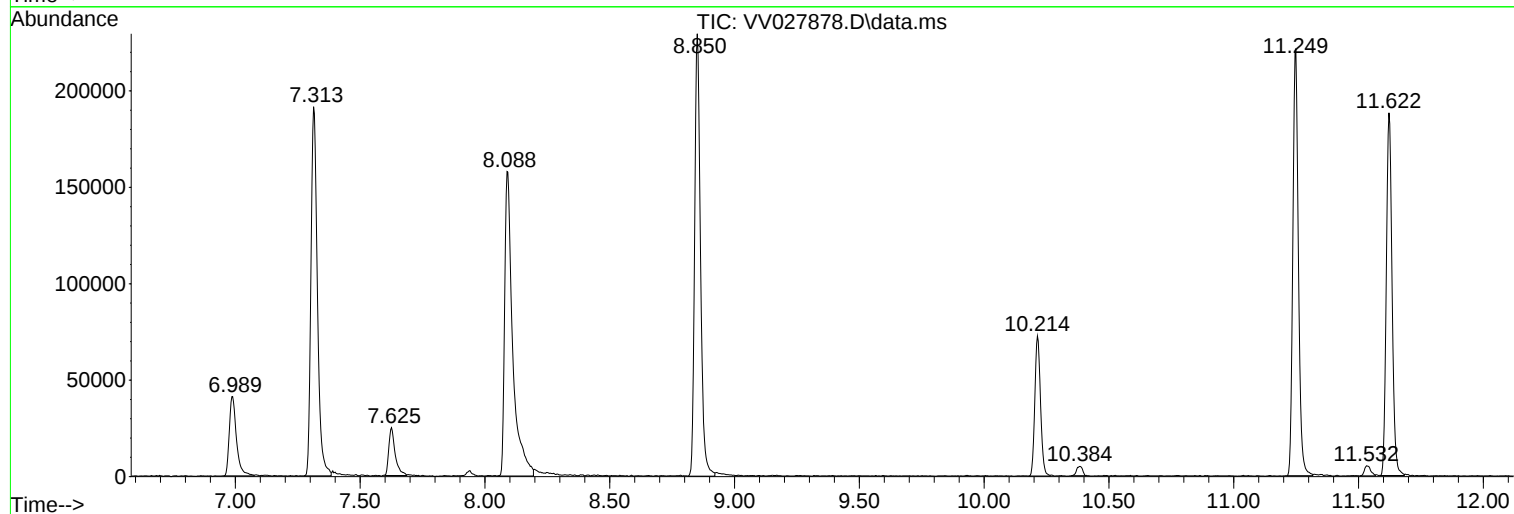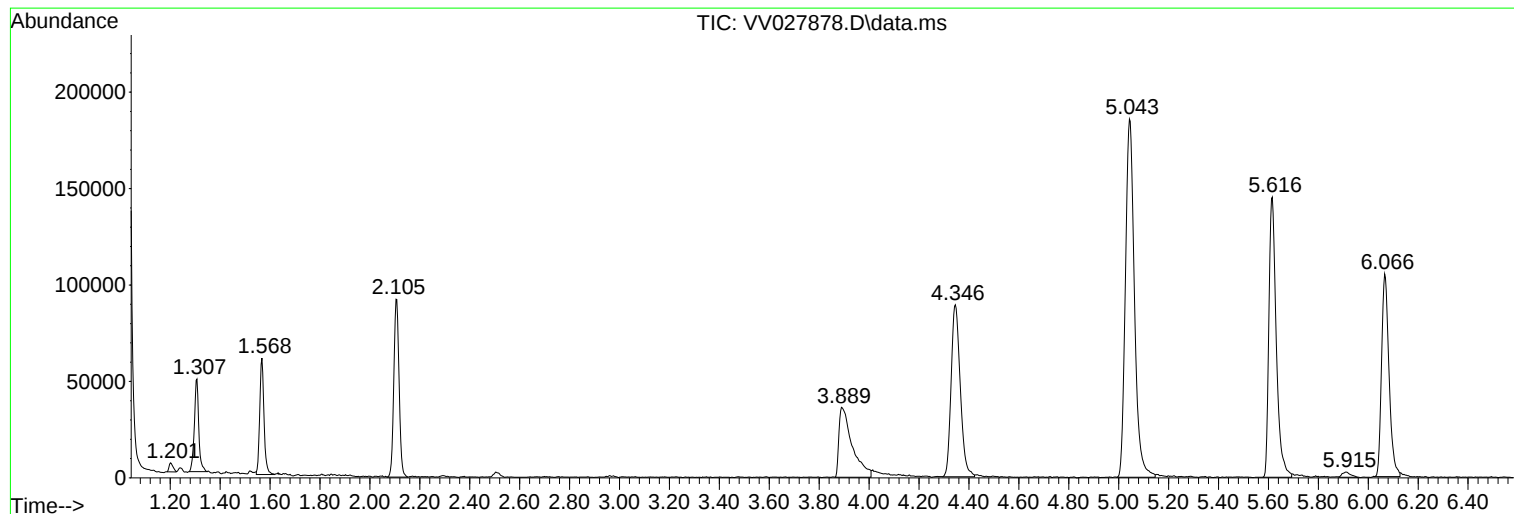

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027878.D
Acq On : 16 Sep 2022 13:37
Operator : SY/MD
Sample : N4618-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027878.D
Acq On : 16 Sep 2022 13:37
Operator : SY/MD
Sample : N4618-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------