

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
 Data File : VV027880.D
 Acq On : 16 Sep 2022 14:26
 Operator : SY/MD
 Sample : N4618-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E66

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027880.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.204	46	51	58	rBV2	9366	9015	1.98%	0.242%
2	1.307	74	83	95	rBV	45387	55574	12.21%	1.490%
3	1.568	157	164	178	rVB	56652	68015	14.95%	1.824%
4	2.108	322	332	346	rVB	85907	123822	27.21%	3.320%
5	2.510	448	457	467	rBV4	3895	6562	1.44%	0.176%
6	3.895	878	888	923	rBV	37770	152505	33.51%	4.090%
7	4.346	1011	1028	1050	rBV	90505	231423	50.85%	6.206%
8	5.043	1230	1245	1282	rBV3	176951	455076	100.00%	12.203%
9	5.616	1408	1423	1451	rBV	147293	306606	67.37%	8.222%
10	6.069	1546	1564	1590	rBV	105714	222428	48.88%	5.965%
11	6.989	1840	1850	1879	rBV2	41514	83454	18.34%	2.238%
12	7.317	1940	1952	1975	rBV	184286	335135	73.64%	8.987%
13	7.625	2038	2048	2063	rBV2	24655	46136	10.14%	1.237%
14	8.091	2183	2193	2226	rBV2	187732	417262	91.69%	11.189%
15	8.850	2418	2429	2459	rBV	231622	387322	85.11%	10.387%
16	10.214	2843	2853	2871	rBV	77742	125018	27.47%	3.353%
17	10.384	2897	2906	2915	rVB2	4131	5689	1.25%	0.153%
18	11.249	3164	3175	3198	rBV	231187	365763	80.37%	9.808%
19	11.532	3250	3263	3279	rBV3	14208	24742	5.44%	0.663%
20	11.622	3279	3291	3310	rVV	196666	307527	67.58%	8.247%




Sum of corrected areas: 3729074

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027880.D
Acq On : 16 Sep 2022 14:26
Operator : SY/MD
Sample : N4618-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

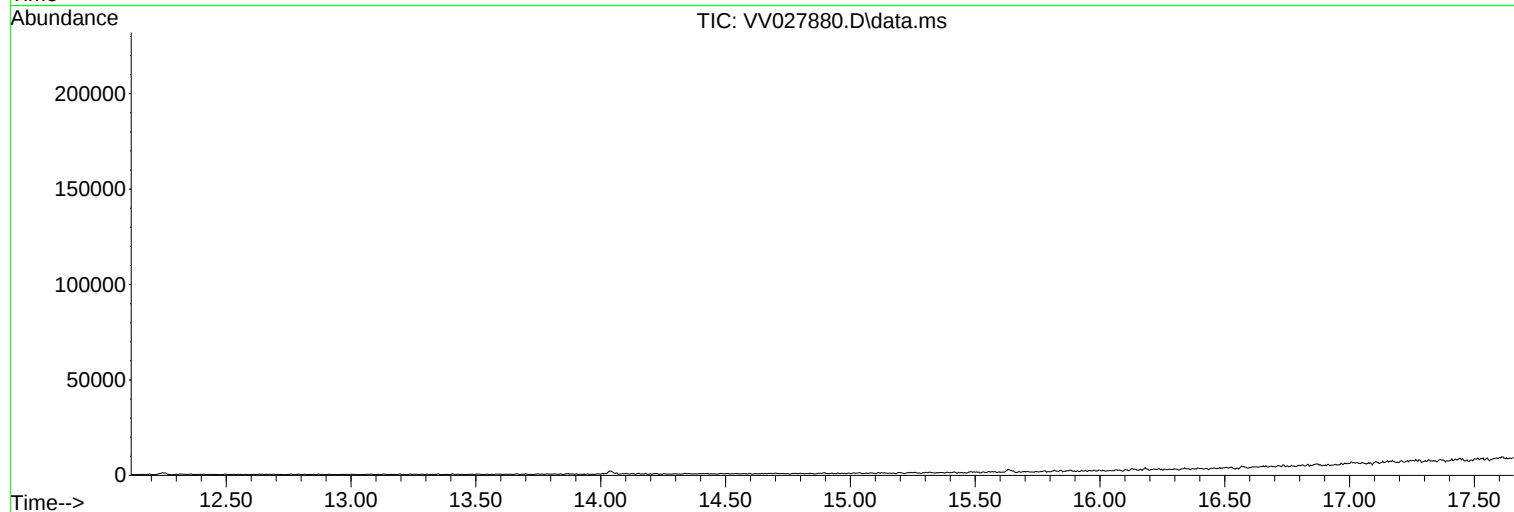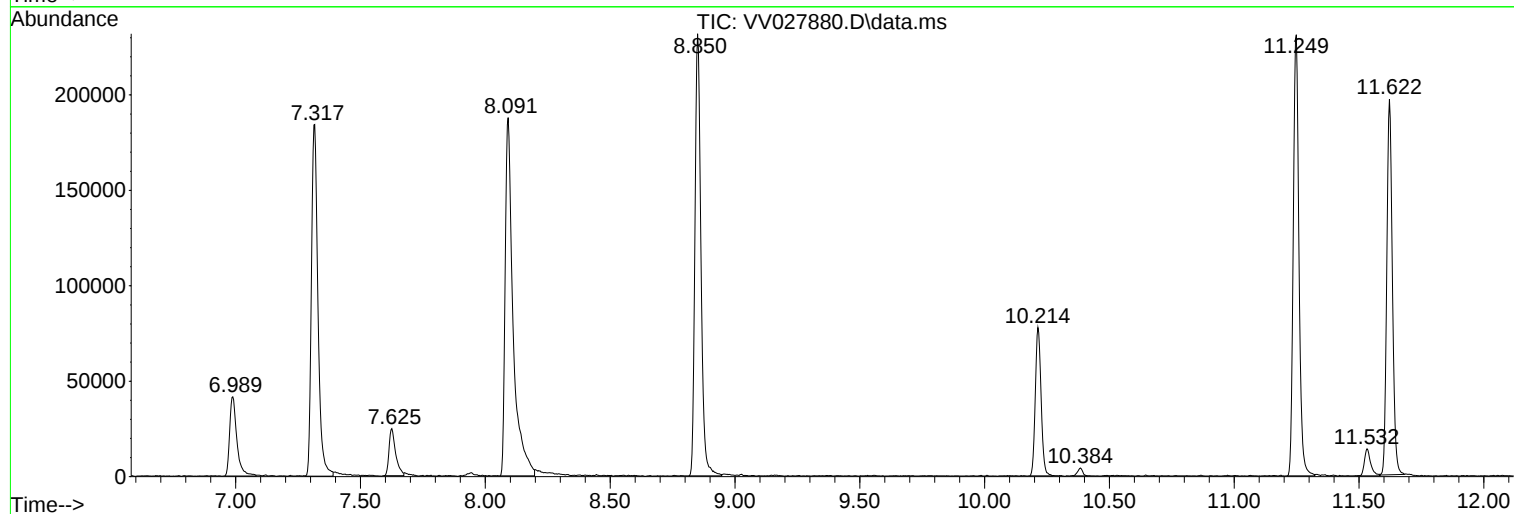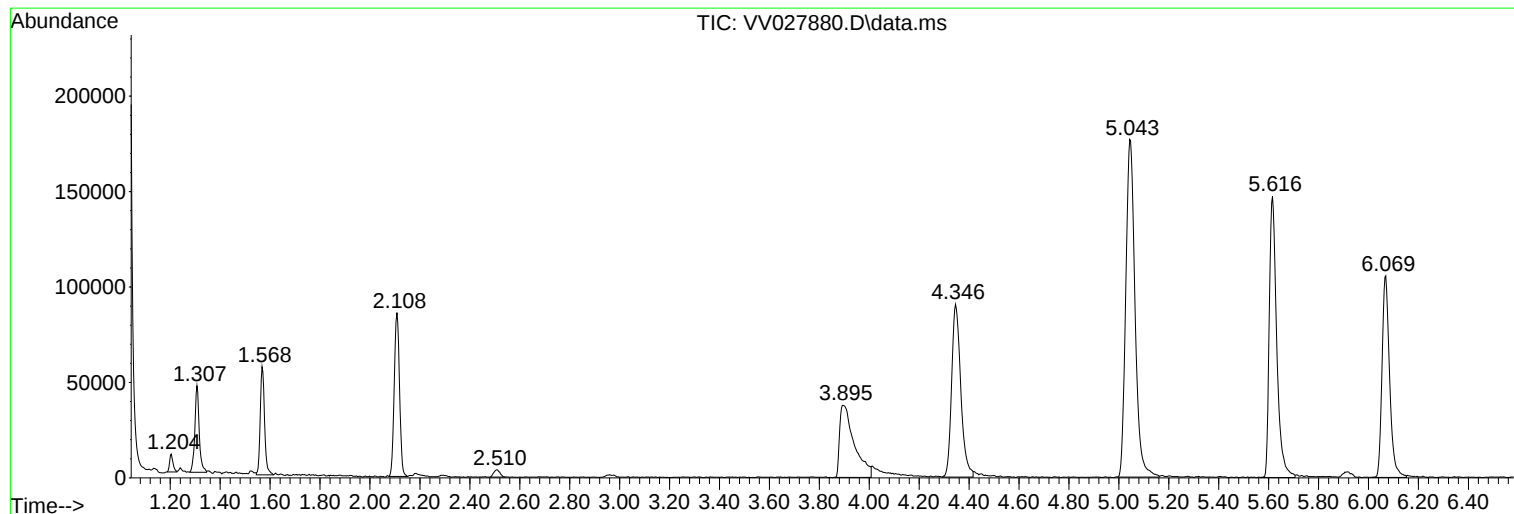

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027880.D
Acq On : 16 Sep 2022 14:26
Operator : SY/MD
Sample : N4618-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027880.D
Acq On : 16 Sep 2022 14:26
Operator : SY/MD
Sample : N4618-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
