

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
 Data File : VV027886.D
 Acq On : 16 Sep 2022 17:15
 Operator : SY/MD
 Sample : N4658-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E75

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027886.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.204	45	51	59	rBV	6959	7553	1.63%	0.198%
2	1.307	73	83	96	rBV	45212	54584	11.76%	1.432%
3	1.568	156	164	177	rBV	50716	60319	13.00%	1.582%
4	2.108	321	332	346	rBV	91972	134706	29.03%	3.534%
5	3.896	878	888	930	rBV2	41508	163014	35.13%	4.276%
6	4.346	1009	1028	1055	rBV2	90349	244233	52.64%	6.407%
7	5.043	1229	1245	1278	rBV2	181663	463974	100.00%	12.172%
8	5.616	1411	1423	1453	rBV	144660	307217	66.21%	8.059%
9	5.918	1504	1517	1543	rVB7	12244	29673	6.40%	0.778%
10	6.066	1550	1563	1592	rBV2	105878	227799	49.10%	5.976%
11	6.989	1840	1850	1870	rBV	41820	82187	17.71%	2.156%
12	7.313	1940	1951	1974	rBV	188718	344474	74.24%	9.037%
13	7.625	2038	2048	2071	rBV2	25833	48830	10.52%	1.281%
14	8.092	2180	2193	2224	rBV2	188053	422688	91.10%	11.089%
15	8.850	2418	2429	2457	rBV	232952	389534	83.96%	10.219%
16	10.214	2842	2853	2866	rBV2	77917	125283	27.00%	3.287%
17	10.378	2897	2904	2915	rBV4	3696	5947	1.28%	0.156%
18	11.246	3164	3174	3193	rBV	233311	368575	79.44%	9.669%
19	11.532	3253	3263	3277	rBV2	11990	20506	4.42%	0.538%
20	11.622	3280	3291	3310	rVV	196426	310775	66.98%	8.153%




Sum of corrected areas: 3811871

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027886.D
Acq On : 16 Sep 2022 17:15
Operator : SY/MD
Sample : N4658-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

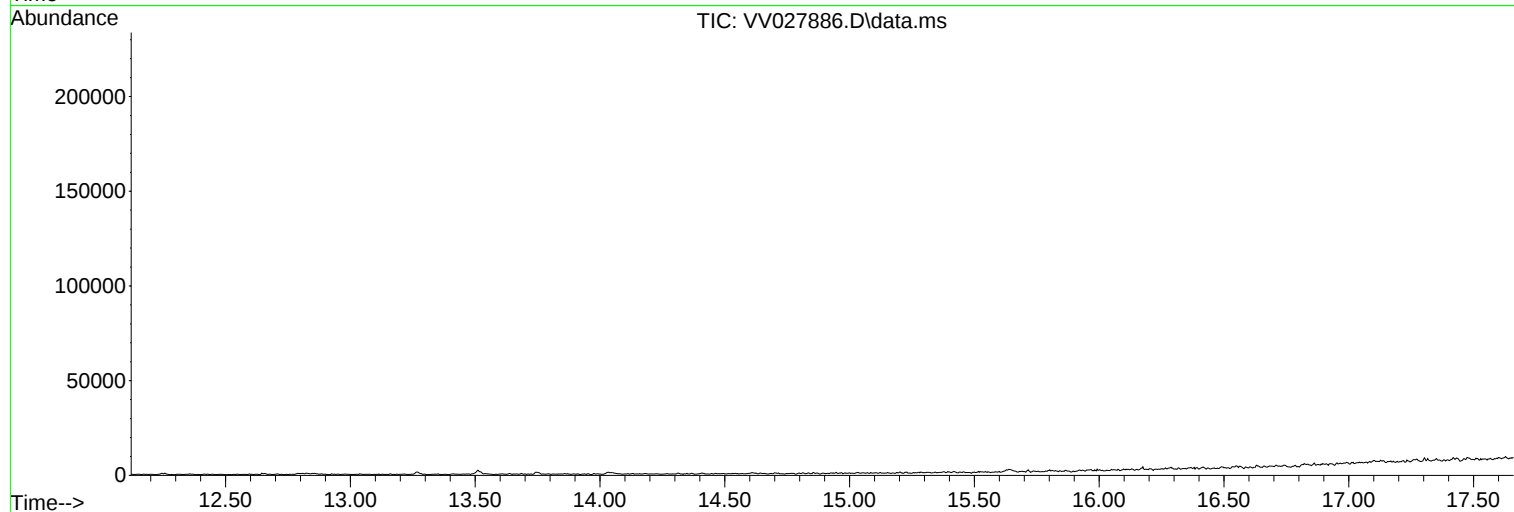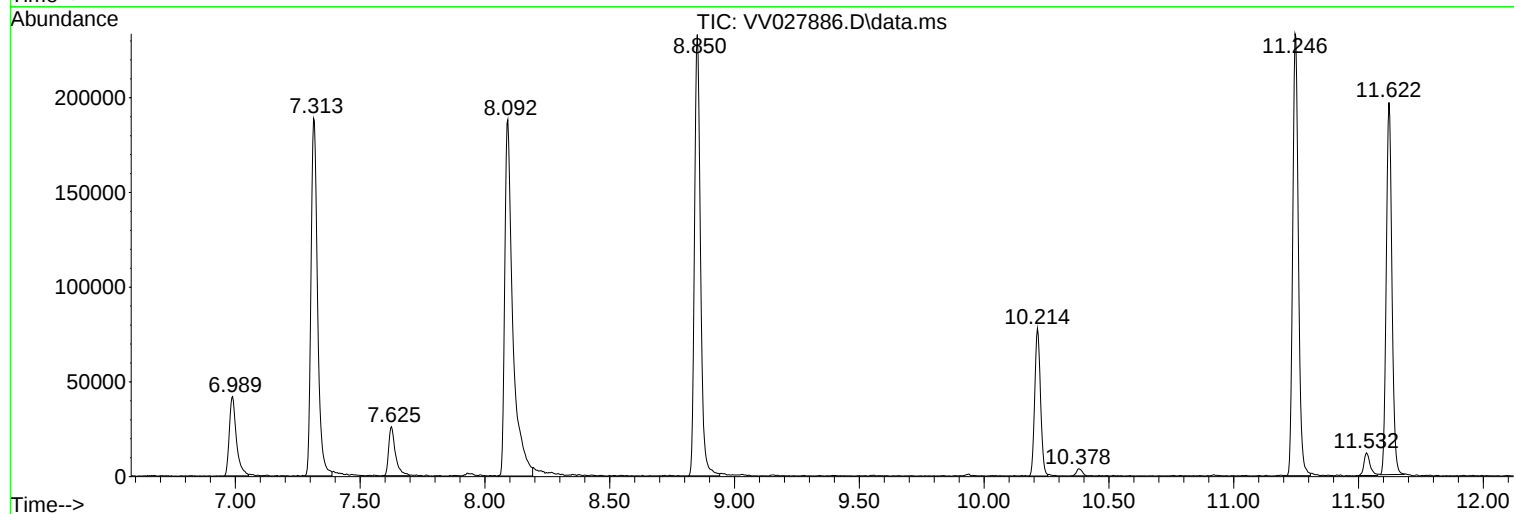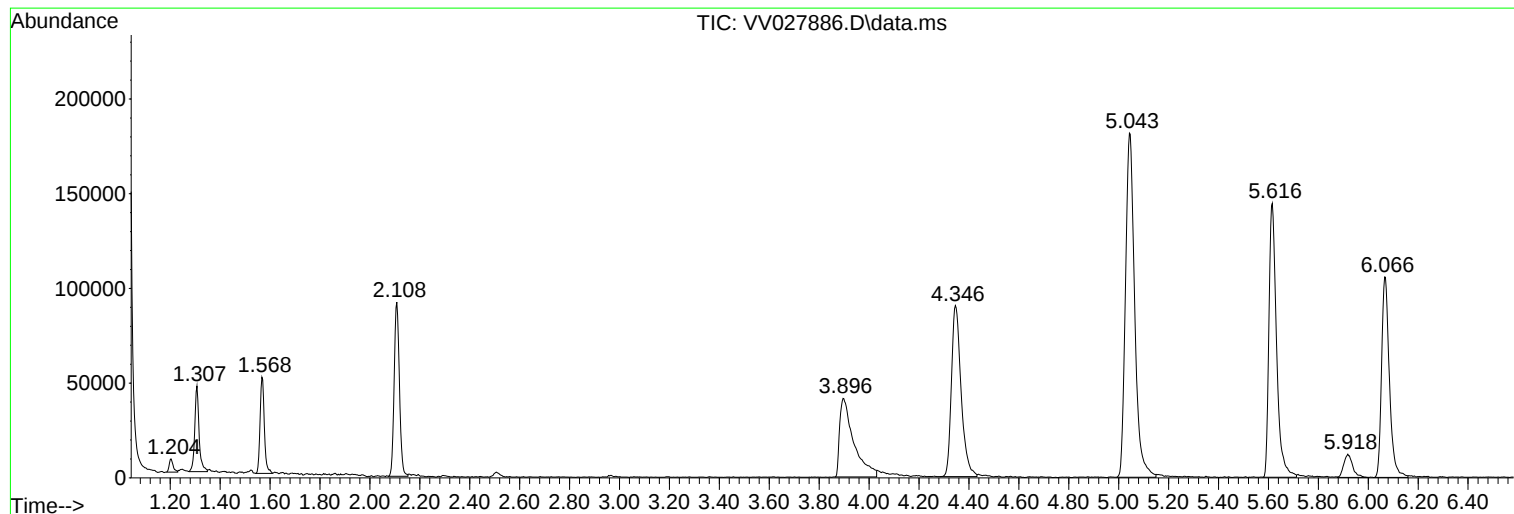

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027886.D
Acq On : 16 Sep 2022 17:15
Operator : SY/MD
Sample : N4658-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027886.D
Acq On : 16 Sep 2022 17:15
Operator : SY/MD
Sample : N4658-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc