

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
 Data File : VV027888.D
 Acq On : 16 Sep 2022 18:03
 Operator : SY/MD
 Sample : N4658-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E81

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027888.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	98	rBV	44874	51941	10.93%	1.348%
2	1.568	157	164	178	rBV	53938	64170	13.50%	1.666%
3	2.108	317	332	346	rBV	102425	149298	31.41%	3.875%
4	3.896	878	888	918	rBV2	41761	152492	32.09%	3.958%
5	4.349	1008	1029	1059	rBV3	94359	269395	56.68%	6.993%
6	5.043	1229	1245	1279	rBV3	184365	475264	100.00%	12.336%
7	5.616	1411	1423	1452	rBV2	144940	304346	64.04%	7.900%
8	6.066	1551	1563	1588	rBV2	108130	227777	47.93%	5.912%
9	6.985	1840	1849	1875	rBV	44708	84926	17.87%	2.204%
10	7.317	1936	1952	1976	rBV	193603	350172	73.68%	9.089%
11	7.625	2039	2048	2066	rBV2	25014	46977	9.88%	1.219%
12	7.937	2133	2145	2157	rBV4	2746	5254	1.11%	0.136%
13	8.091	2182	2193	2227	rBV2	191583	431738	90.84%	11.206%
14	8.850	2418	2429	2456	rBV	229541	385968	81.21%	10.018%
15	10.214	2842	2853	2870	rBV2	77664	123427	25.97%	3.204%
16	10.381	2893	2905	2917	rBV3	9190	14372	3.02%	0.373%
17	11.249	3164	3175	3196	rBV	233803	370376	77.93%	9.614%
18	11.535	3254	3264	3278	rBV4	12602	23192	4.88%	0.602%
19	11.622	3280	3291	3307	rVV	200663	321483	67.64%	8.345%




Sum of corrected areas: 3852568

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027888.D
Acq On : 16 Sep 2022 18:03
Operator : SY/MD
Sample : N4658-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

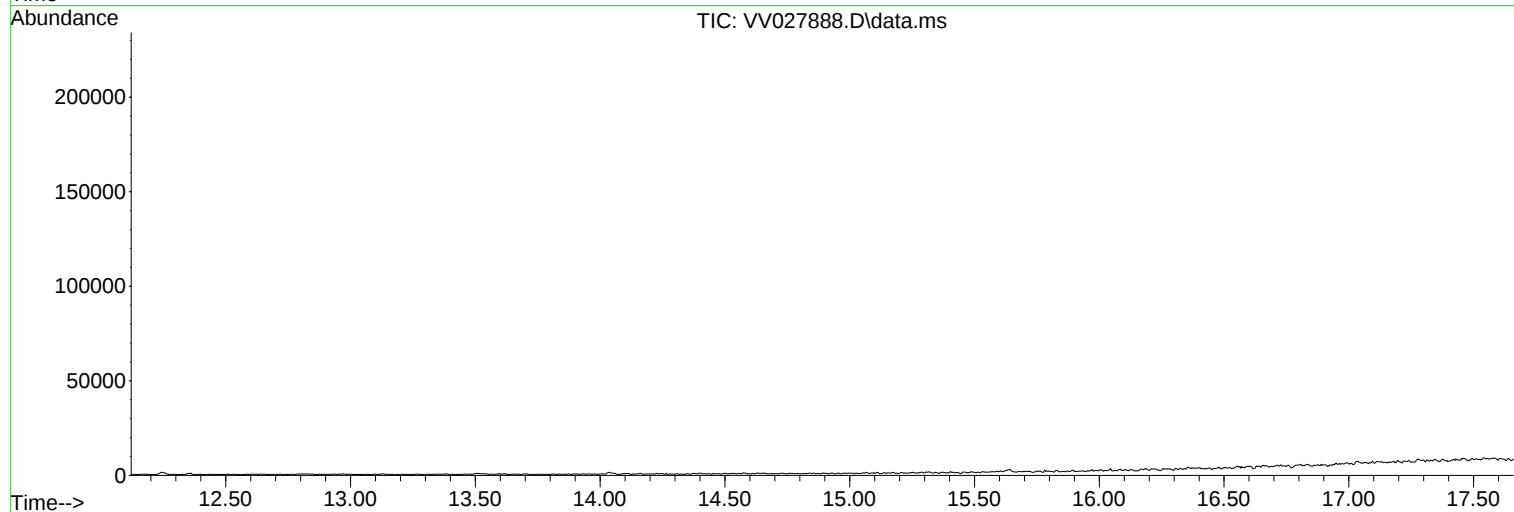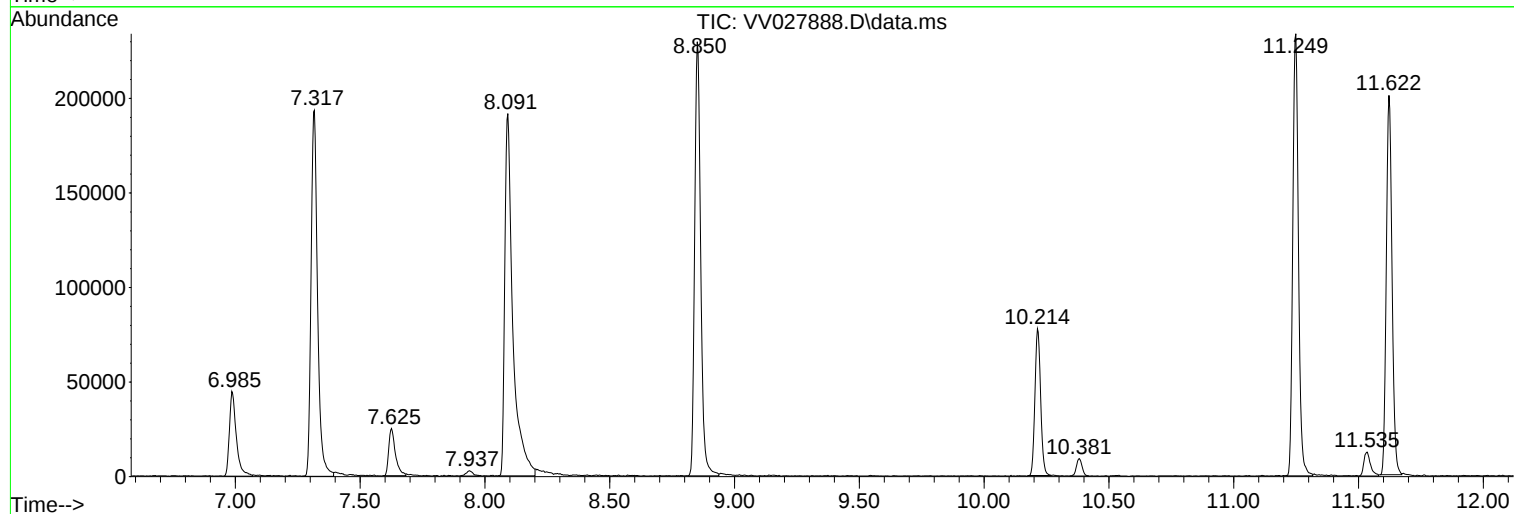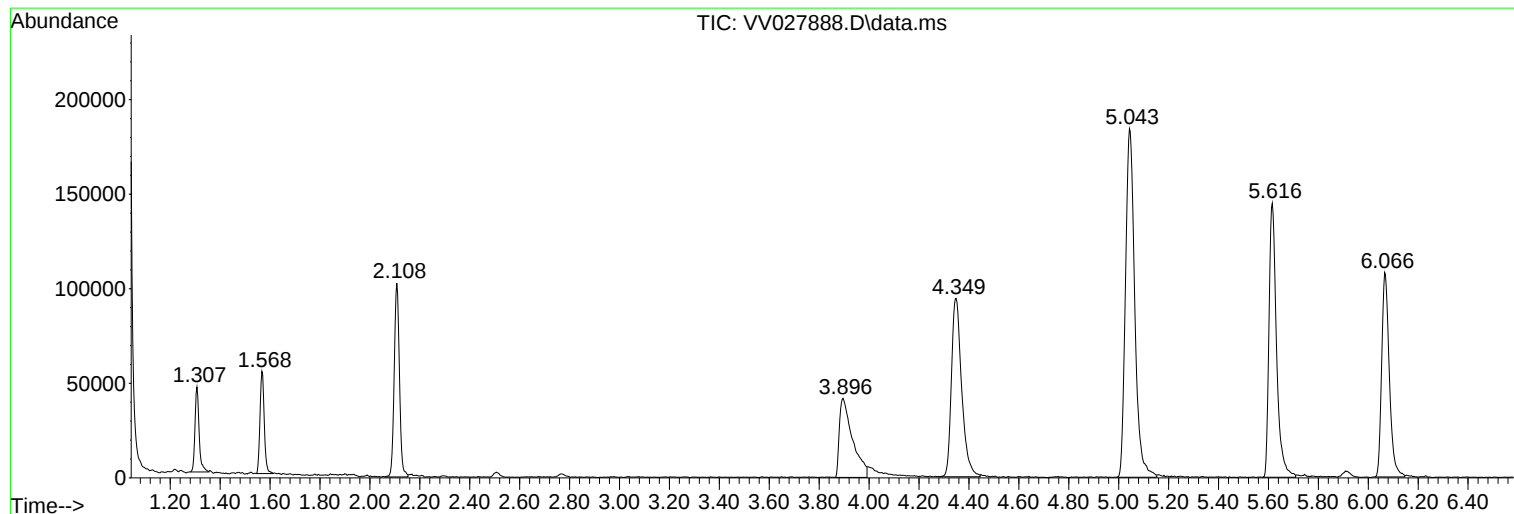

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027888.D
Acq On : 16 Sep 2022 18:03
Operator : SY/MD
Sample : N4658-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027888.D
Acq On : 16 Sep 2022 18:03
Operator : SY/MD
Sample : N4658-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E81

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc