

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
 Data File : VV027891.D
 Acq On : 16 Sep 2022 19:16
 Operator : SY/MD
 Sample : N4672-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EB8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027891.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	96	rBV	42769	48502	11.35%	1.382%
2	1.568	156	164	178	rBV	53577	62633	14.66%	1.784%
3	2.108	321	332	345	rBV	92689	134445	31.47%	3.829%
4	3.892	877	887	923	rBV	39981	145866	34.15%	4.155%
5	4.346	1011	1028	1063	rVB	84285	216445	50.67%	6.165%
6	5.043	1229	1245	1270	rBV4	164453	427158	100.00%	12.167%
7	5.616	1410	1423	1454	rBV	131502	276264	64.67%	7.869%
8	5.911	1505	1515	1529	rVB8	2998	6952	1.63%	0.198%
9	6.066	1551	1563	1586	rBV	100615	209601	49.07%	5.970%
10	6.989	1837	1850	1870	rBV	38603	75398	17.65%	2.148%
11	7.313	1939	1951	1972	rBV	176980	317604	74.35%	9.046%
12	7.625	2039	2048	2067	rBV2	23211	45225	10.59%	1.288%
13	7.937	2136	2145	2157	rBV3	2525	4540	1.06%	0.129%
14	8.091	2183	2193	2222	rBV2	174165	393527	92.13%	11.209%
15	8.850	2418	2429	2455	rBV	213531	356012	83.34%	10.140%
16	10.214	2840	2853	2868	rBV	73663	118247	27.68%	3.368%
17	10.381	2895	2905	2918	rBV2	7288	11785	2.76%	0.336%
18	11.246	3163	3174	3196	rBV	216902	341142	79.86%	9.717%
19	11.535	3255	3264	3278	rBV4	7882	14157	3.31%	0.403%
20	11.622	3280	3291	3306	rBV	189770	300190	70.28%	8.550%
21	12.349	3511	3517	3529	rBV6	3397	5102	1.19%	0.145%




Sum of corrected areas: 3510795

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027891.D
Acq On : 16 Sep 2022 19:16
Operator : SY/MD
Sample : N4672-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EB8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

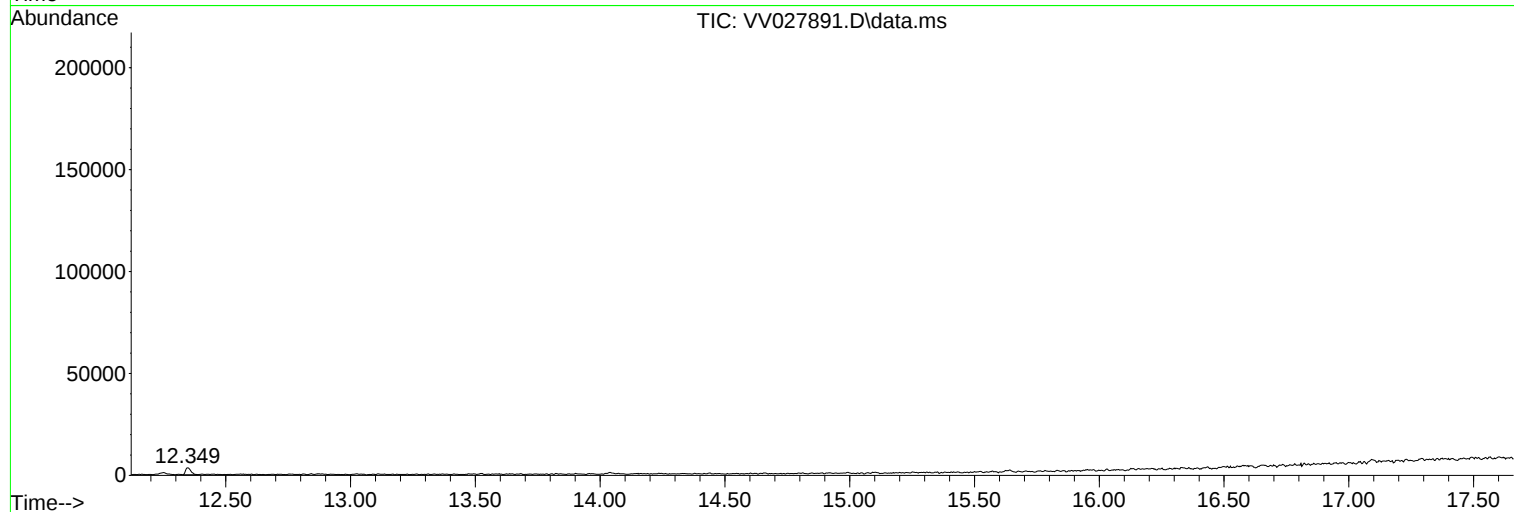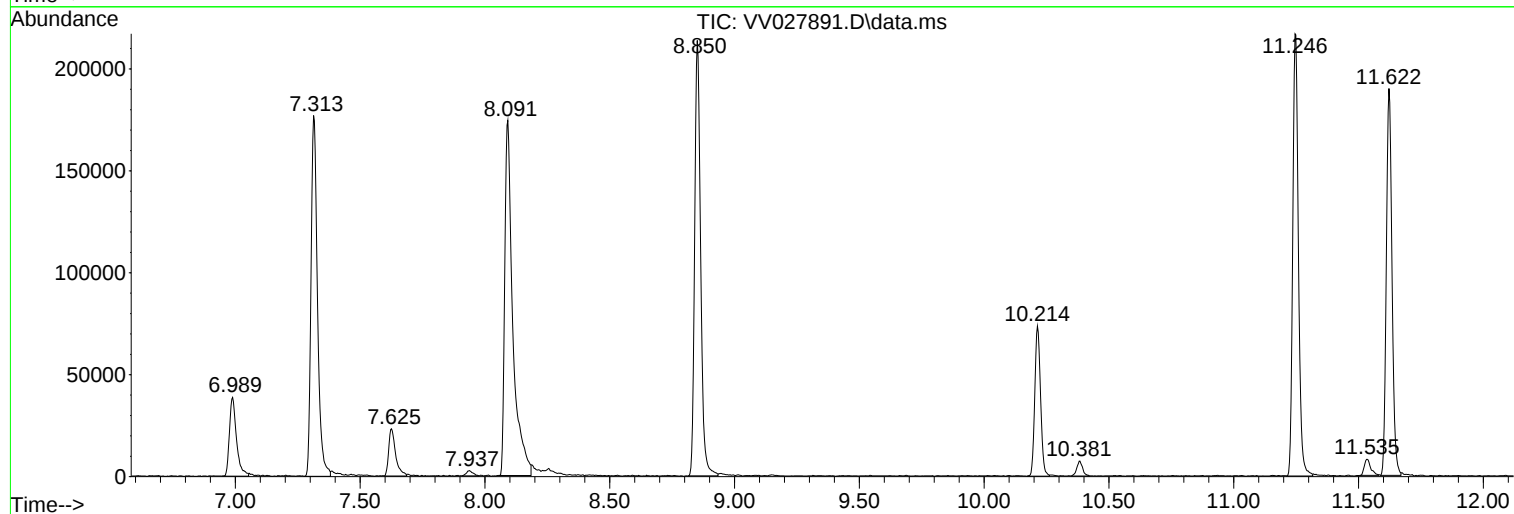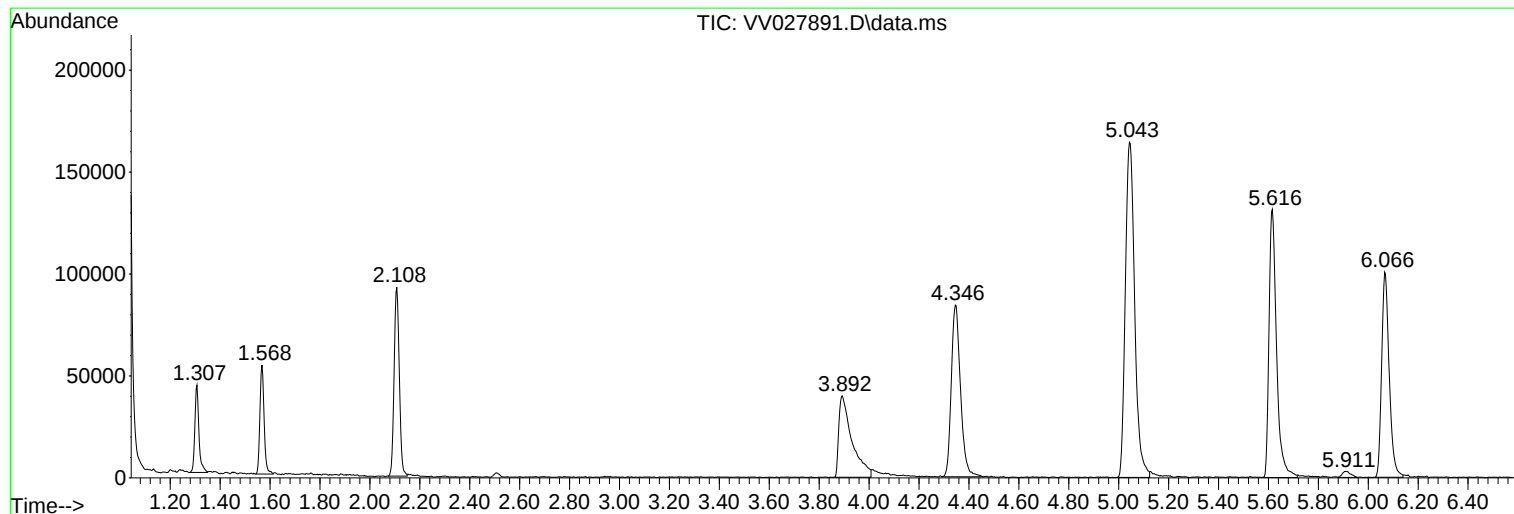

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027891.D
Acq On : 16 Sep 2022 19:16
Operator : SY/MD
Sample : N4672-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EB8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027891.D
Acq On : 16 Sep 2022 19:16
Operator : SY/MD
Sample : N4672-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EB8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------