

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
 Data File : VV027892.D
 Acq On : 16 Sep 2022 19:41
 Operator : SY/MD
 Sample : N4672-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EB9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027892.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	95	rBV	45367	51621	11.30%	1.382%
2	1.568	156	164	175	rBV	52132	60722	13.29%	1.626%
3	2.108	321	332	346	rBV	89320	130529	28.57%	3.495%
4	3.889	877	886	917	rBV2	41642	150449	32.93%	4.029%
5	4.346	1012	1028	1054	rBV2	89686	228006	49.91%	6.106%
6	5.043	1227	1245	1273	rBV3	180337	456859	100.00%	12.234%
7	5.616	1410	1423	1456	rBV	141259	299817	65.63%	8.029%
8	5.911	1504	1515	1531	rVB6	3768	8911	1.95%	0.239%
9	6.066	1549	1563	1590	rBV2	107310	225218	49.30%	6.031%
10	6.985	1840	1849	1866	rBV2	41472	78795	17.25%	2.110%
11	7.313	1940	1951	1972	rBV	187840	337723	73.92%	9.044%
12	7.625	2035	2048	2067	rBV	25677	47602	10.42%	1.275%
13	7.940	2136	2146	2157	rBV3	2663	5094	1.12%	0.136%
14	8.091	2178	2193	2228	rBV2	181884	424066	92.82%	11.356%
15	8.850	2412	2429	2459	rBV	227022	386818	84.67%	10.359%
16	10.214	2842	2853	2869	rBV	78814	124028	27.15%	3.321%
17	10.381	2895	2905	2917	rVB	7991	12708	2.78%	0.340%
18	11.246	3161	3174	3201	rBV	232323	369204	80.81%	9.887%
19	11.535	3255	3264	3275	rBV3	9856	16673	3.65%	0.446%
20	11.622	3280	3291	3317	rVV	199207	319413	69.92%	8.554%




Sum of corrected areas: 3734256

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027892.D
Acq On : 16 Sep 2022 19:41
Operator : SY/MD
Sample : N4672-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

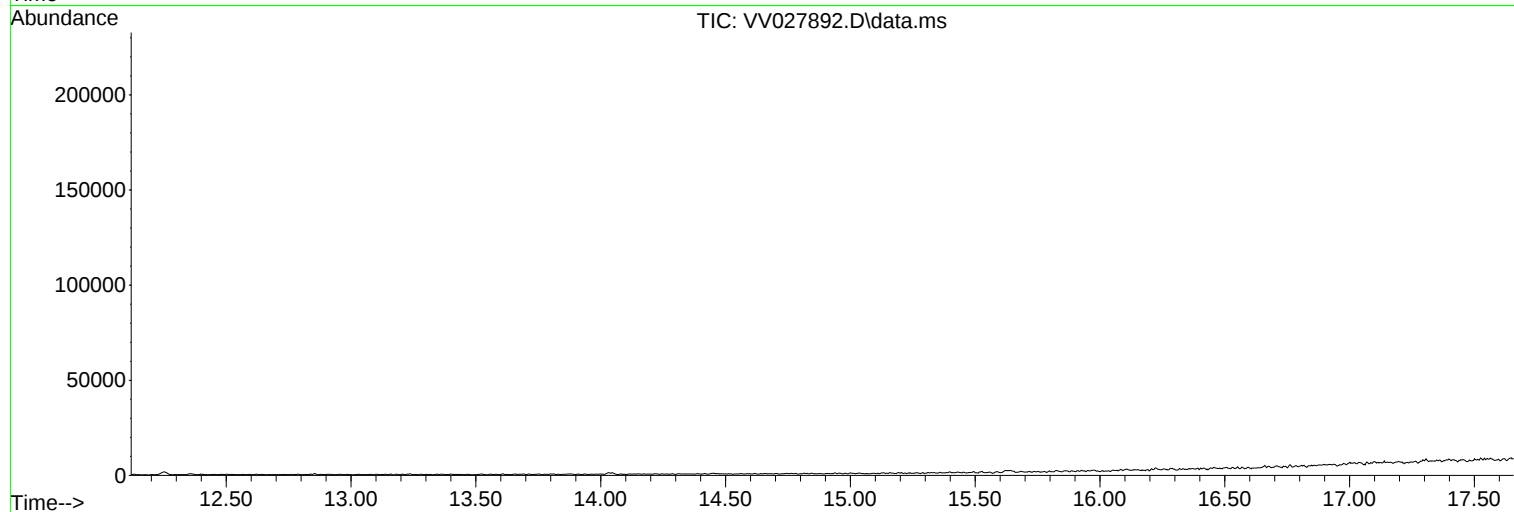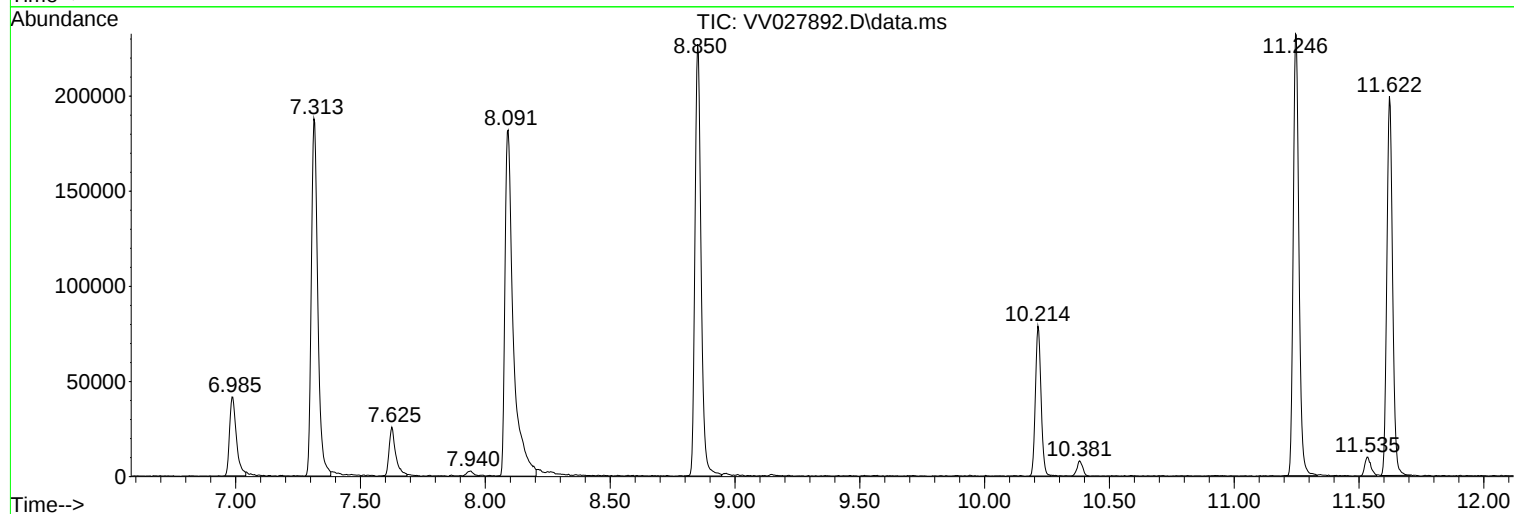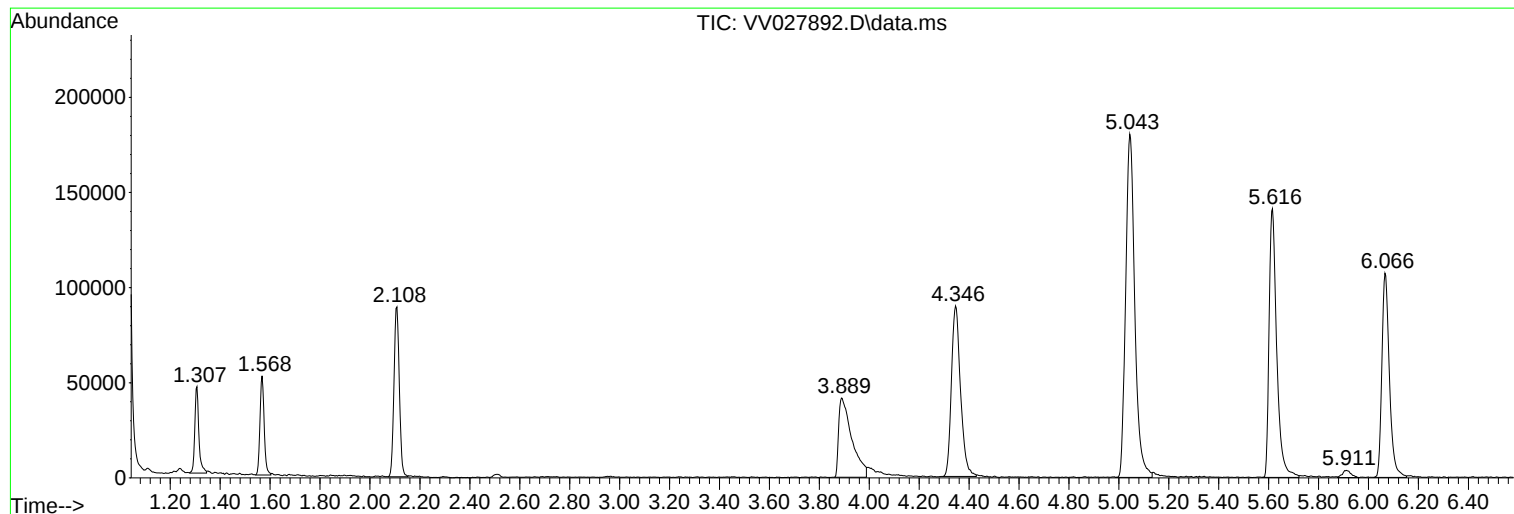

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027892.D
Acq On : 16 Sep 2022 19:41
Operator : SY/MD
Sample : N4672-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027892.D
Acq On : 16 Sep 2022 19:41
Operator : SY/MD
Sample : N4672-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
