

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
 Data File : VV027893.D
 Acq On : 16 Sep 2022 20:05
 Operator : SY/MD
 Sample : N4672-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027893.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	72	82	101	rVB	45784	55974	12.52%	1.510%
2	1.564	155	163	177	rBV	52418	61625	13.78%	1.662%
3	2.105	321	331	347	rBV	87498	128078	28.64%	3.454%
4	3.889	876	886	915	rBV2	42444	147623	33.02%	3.981%
5	4.342	1011	1027	1055	rBV2	86751	219472	49.08%	5.919%
6	5.043	1230	1245	1276	rBV3	171960	447132	100.00%	12.059%
7	5.612	1411	1422	1449	rBV	129289	272307	60.90%	7.344%
8	5.905	1503	1513	1517	rBV4	4115	6272	1.40%	0.169%
9	6.066	1551	1563	1591	rBV2	103102	217331	48.61%	5.861%
10	6.301	1628	1636	1648	rBV5	5858	13549	3.03%	0.365%
11	6.985	1840	1849	1870	rBV2	40744	78241	17.50%	2.110%
12	7.313	1941	1951	1966	rBV	183036	323346	72.32%	8.721%
13	7.391	1966	1975	1995	rVB	30574	61087	13.66%	1.648%
14	7.622	2038	2047	2072	rBV2	23687	46080	10.31%	1.243%
15	7.940	2132	2146	2159	rBV5	3263	6238	1.40%	0.168%
16	8.088	2183	2192	2222	rBV2	173193	395803	88.52%	10.675%
17	8.246	2235	2241	2257	rVB9	8211	15116	3.38%	0.408%
18	8.850	2419	2429	2454	rBV	215155	358077	80.08%	9.657%
19	9.143	2512	2520	2537	rBV4	4309	7654	1.71%	0.206%
20	9.567	2636	2652	2672	rBV3	15735	29758	6.66%	0.803%
21	10.214	2842	2853	2877	rVB2	74725	120419	26.93%	3.248%
22	10.381	2893	2905	2919	rBV	11344	17598	3.94%	0.475%
23	11.246	3163	3174	3189	rBV	222164	343616	76.85%	9.267%
24	11.532	3255	3263	3279	rBV2	11150	18272	4.09%	0.493%
25	11.622	3280	3291	3310	rVV	195913	310760	69.50%	8.381%
26	12.349	3509	3517	3527	rBV5	4538	6362	1.42%	0.172%




Sum of corrected areas: 3707790

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027893.D
Acq On : 16 Sep 2022 20:05
Operator : SY/MD
Sample : N4672-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

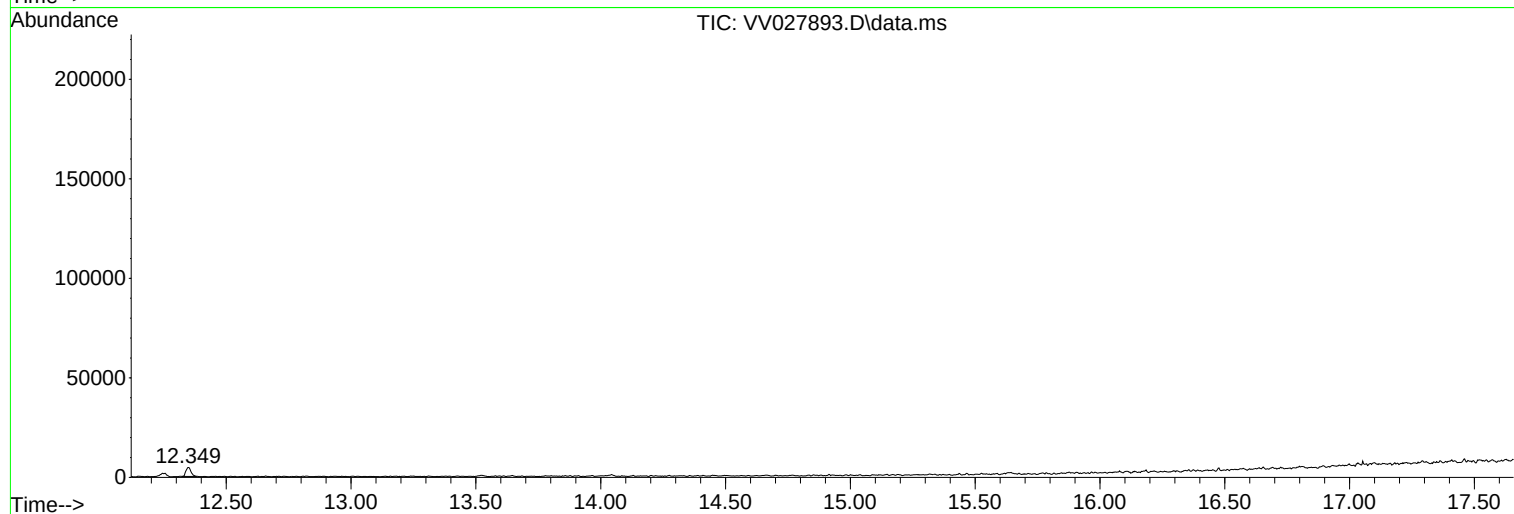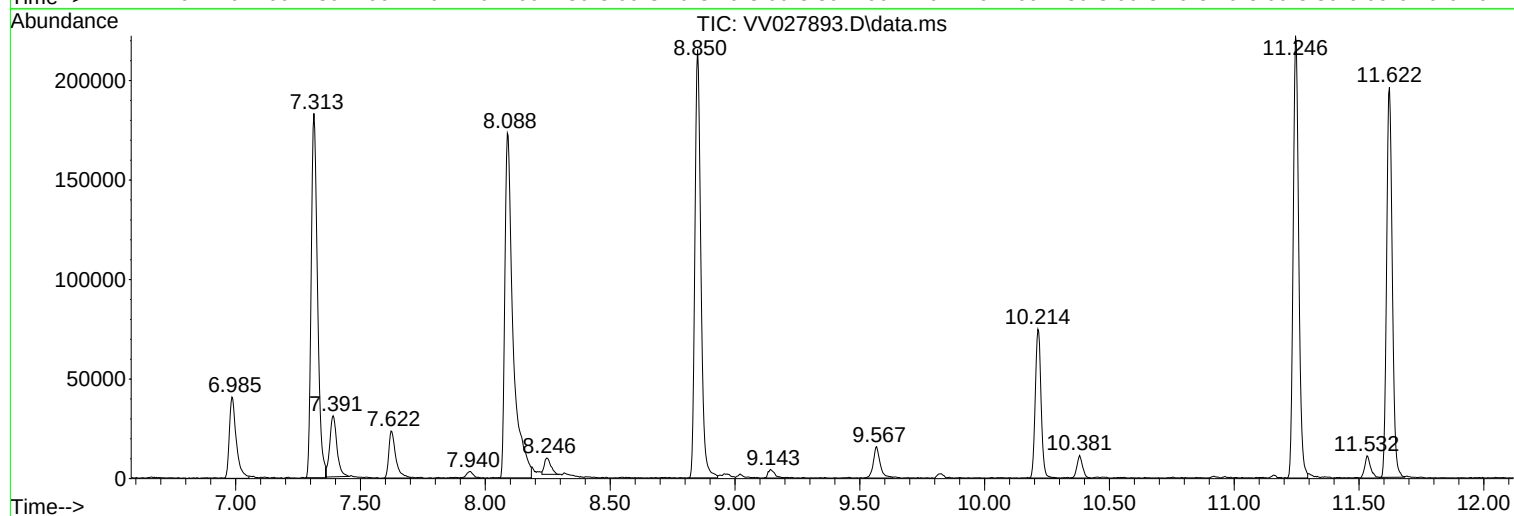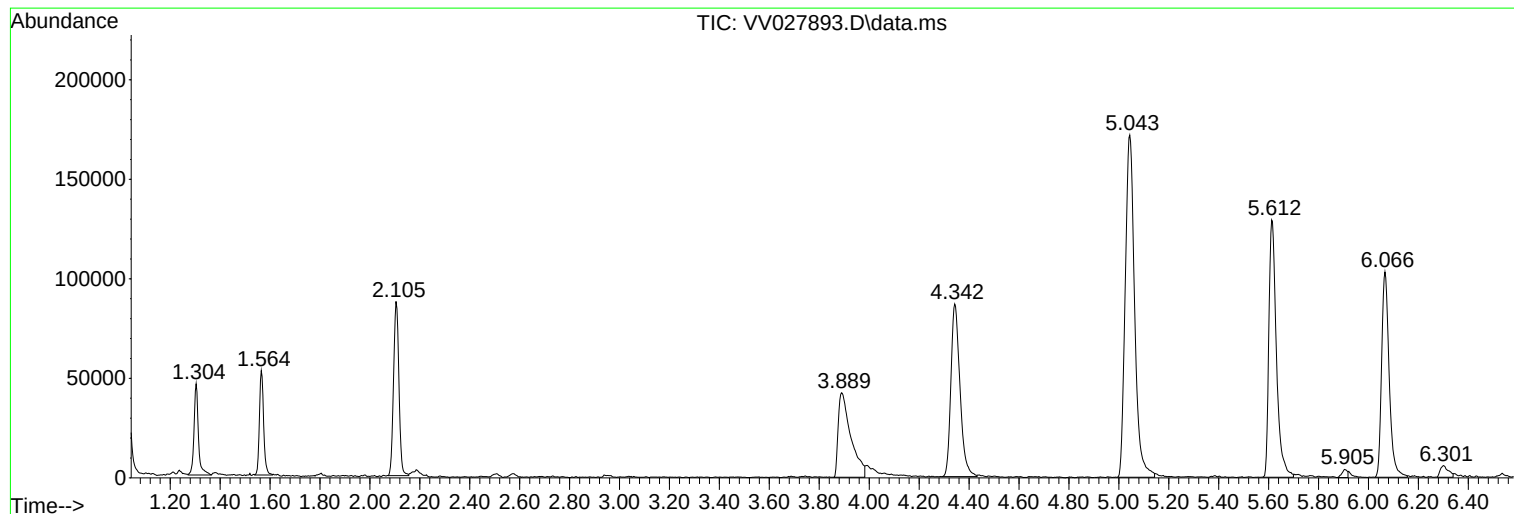

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027893.D
Acq On : 16 Sep 2022 20:05
Operator : SY/MD
Sample : N4672-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027893.D
Acq On : 16 Sep 2022 20:05
Operator : SY/MD
Sample : N4672-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc