

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
 Data File : VV027894.D
 Acq On : 16 Sep 2022 20:30
 Operator : SY/MD
 Sample : N4672-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027894.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	93	rBV	51601	55404	11.27%	1.435%
2	1.568	156	164	178	rBV	54600	64873	13.20%	1.680%
3	2.108	321	332	347	rBV	87605	126627	25.77%	3.279%
4	3.892	876	887	934	rBV	47946	174896	35.59%	4.529%
5	4.346	1012	1028	1057	rBV	96169	242049	49.25%	6.268%
6	5.043	1228	1245	1281	rBV2	190404	491460	100.00%	12.727%
7	5.616	1410	1423	1462	rBV	135197	289154	58.84%	7.488%
8	6.066	1550	1563	1595	rBV2	112441	239188	48.67%	6.194%
9	6.989	1839	1850	1870	rBV2	43803	85321	17.36%	2.209%
10	7.313	1939	1951	1976	rBV	199371	364503	74.17%	9.439%
11	7.625	2038	2048	2067	rBV	26668	49971	10.17%	1.294%
12	7.937	2137	2145	2156	rVB3	3212	5676	1.15%	0.147%
13	8.092	2179	2193	2233	rBV2	192630	452071	91.99%	11.707%
14	8.850	2418	2429	2454	rBV	219579	366378	74.55%	9.488%
15	10.214	2842	2853	2868	rBV	83165	131628	26.78%	3.409%
16	10.381	2894	2905	2917	rVB2	11136	17843	3.63%	0.462%
17	11.246	3163	3174	3196	rBV	226127	353638	71.96%	9.158%
18	11.535	3254	3264	3274	rBV3	6203	9436	1.92%	0.244%
19	11.622	3280	3291	3311	rBV	209731	341557	69.50%	8.845%




Sum of corrected areas: 3861673

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027894.D
Acq On : 16 Sep 2022 20:30
Operator : SY/MD
Sample : N4672-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

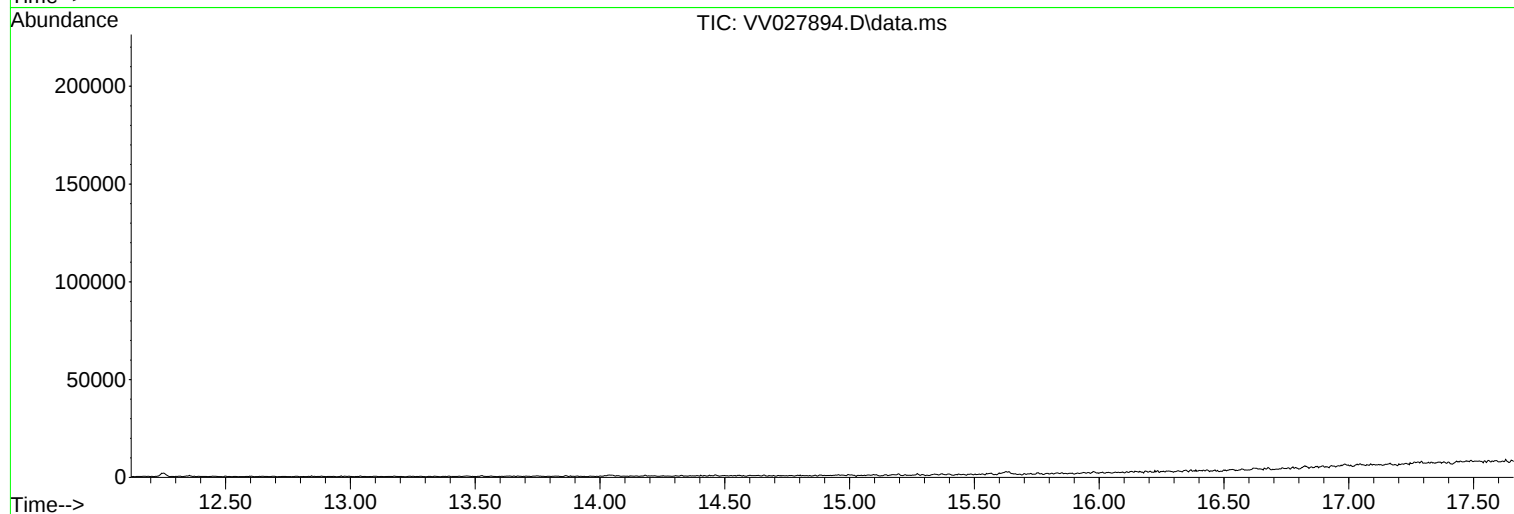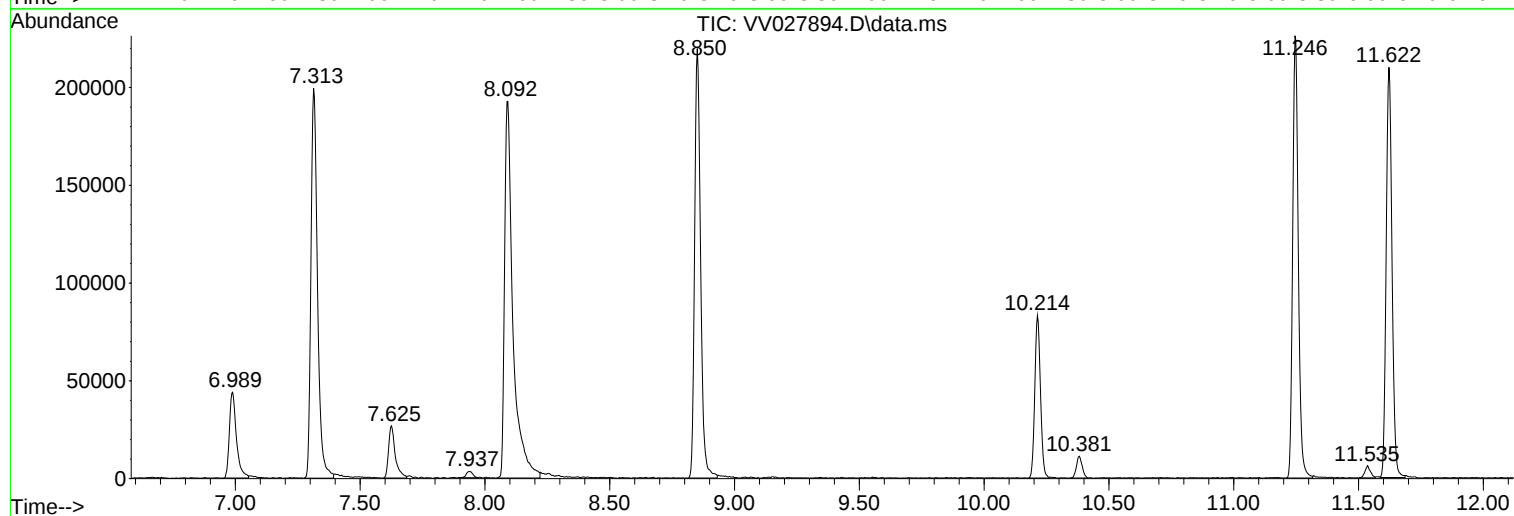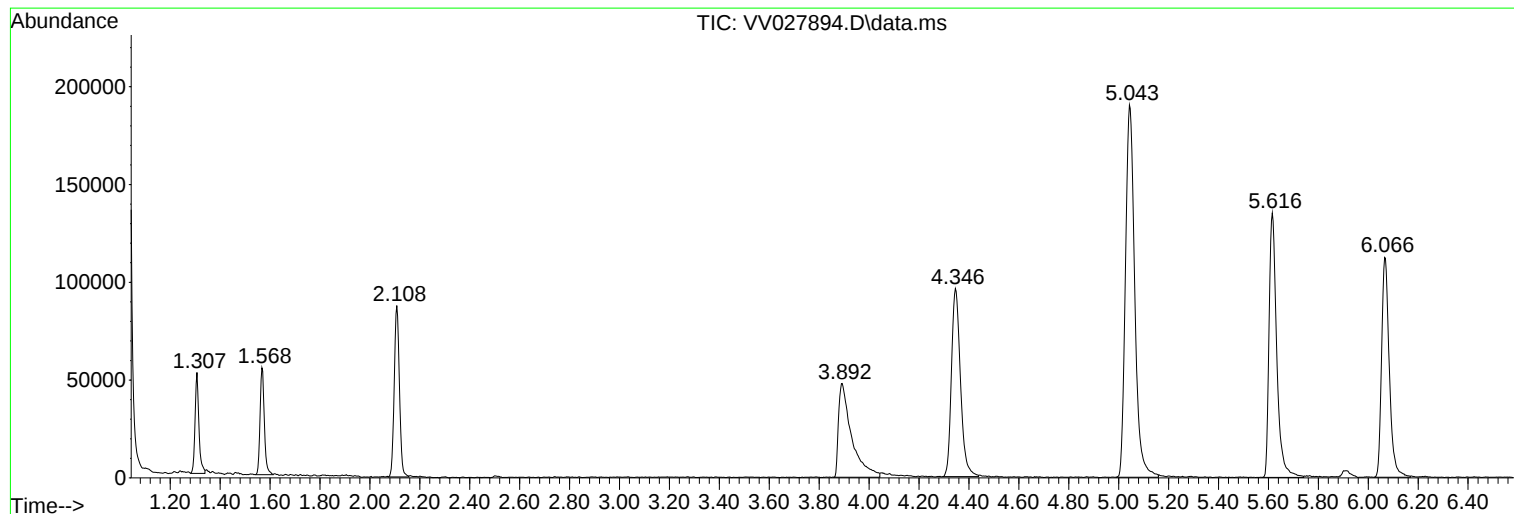

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027894.D
Acq On : 16 Sep 2022 20:30
Operator : SY/MD
Sample : N4672-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027894.D
Acq On : 16 Sep 2022 20:30
Operator : SY/MD
Sample : N4672-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc