

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
 Data File : VV027895.D
 Acq On : 16 Sep 2022 20:53
 Operator : SY/MD
 Sample : N4672-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ED0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027895.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	102	rVB	46432	54758	11.60%	1.430%
2	1.568	156	164	177	rVB	57372	69410	14.70%	1.812%
3	2.108	322	332	344	rBV	100505	144371	30.58%	3.770%
4	3.892	876	887	927	rBV	43569	163486	34.63%	4.269%
5	4.346	1011	1028	1052	rBV	92091	231699	49.08%	6.050%
6	5.047	1230	1246	1275	rBV2	183633	472073	100.00%	12.326%
7	5.616	1412	1423	1448	rBV2	141888	295702	62.64%	7.721%
8	5.915	1505	1516	1526	rBV5	3638	7689	1.63%	0.201%
9	6.069	1551	1564	1583	rBV	109569	228979	48.50%	5.979%
10	6.989	1835	1850	1873	rBV2	42613	84382	17.87%	2.203%
11	7.317	1939	1952	1972	rBV	193499	347642	73.64%	9.077%
12	7.625	2040	2048	2068	rBV2	25303	46719	9.90%	1.220%
13	8.092	2182	2193	2227	rBV2	191102	436322	92.43%	11.393%
14	8.850	2419	2429	2451	rBV	230630	382333	80.99%	9.983%
15	10.217	2843	2854	2871	rBV	80974	129657	27.47%	3.385%
16	10.381	2895	2905	2916	rBV3	8065	12890	2.73%	0.337%
17	11.249	3163	3175	3205	rBV	234278	370465	78.48%	9.673%
18	11.535	3254	3264	3279	rBV3	9671	17316	3.67%	0.452%
19	11.622	3279	3291	3319	rVB	210410	333991	70.75%	8.721%




Sum of corrected areas: 3829884

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027895.D
Acq On : 16 Sep 2022 20:53
Operator : SY/MD
Sample : N4672-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

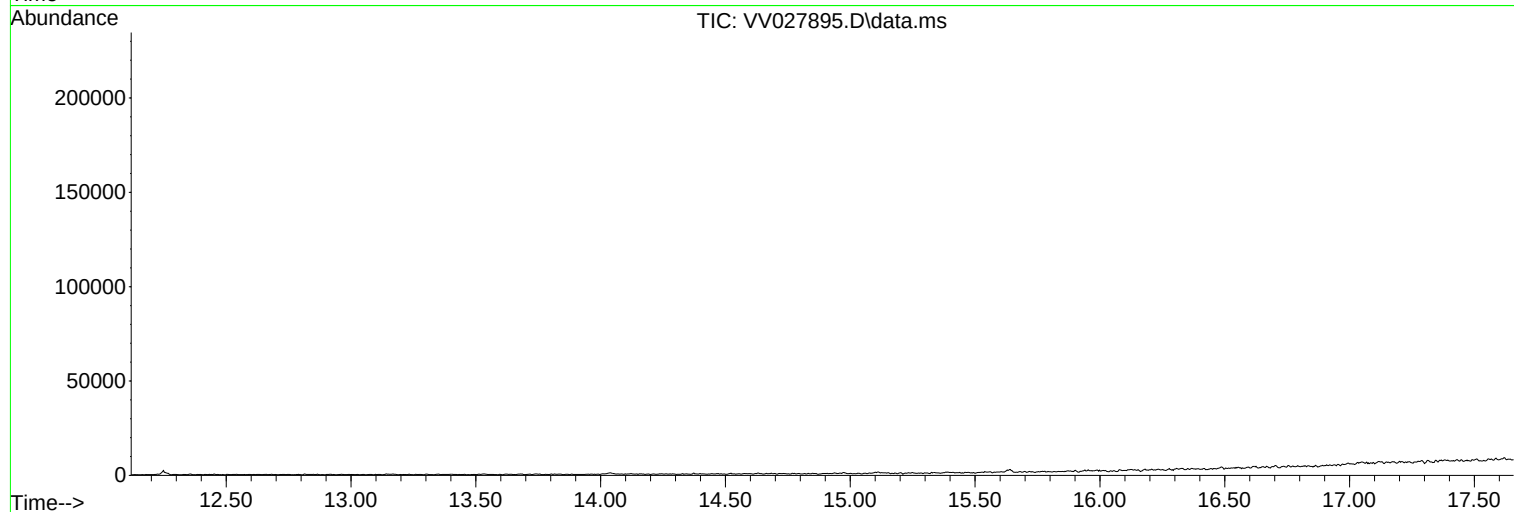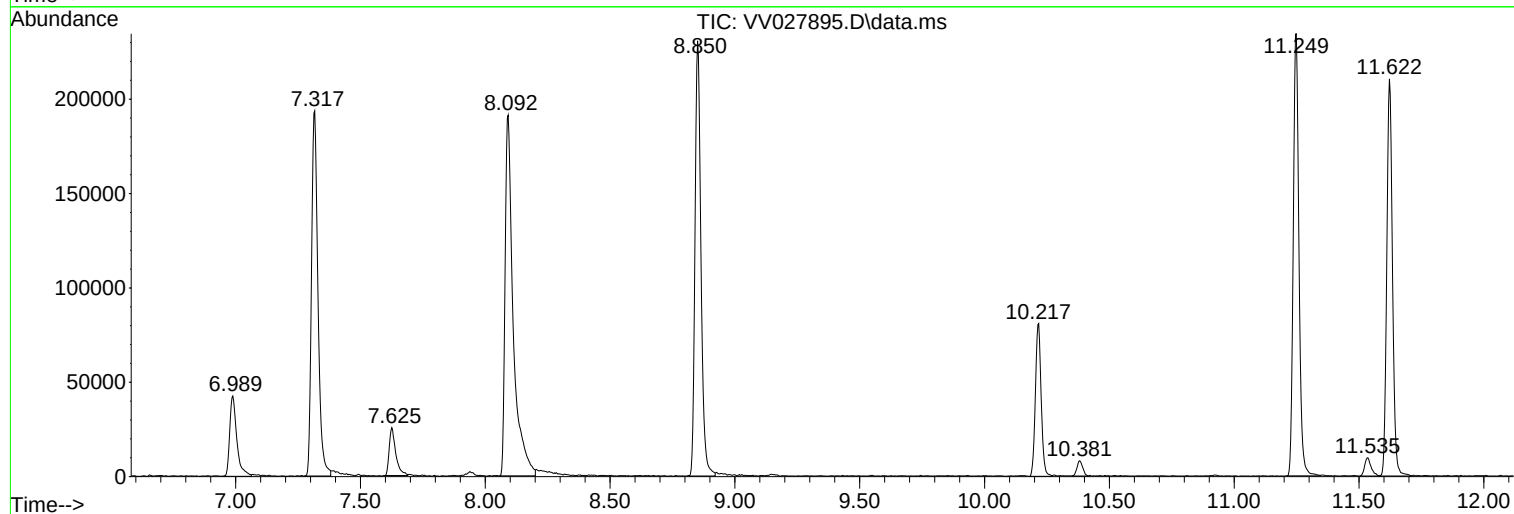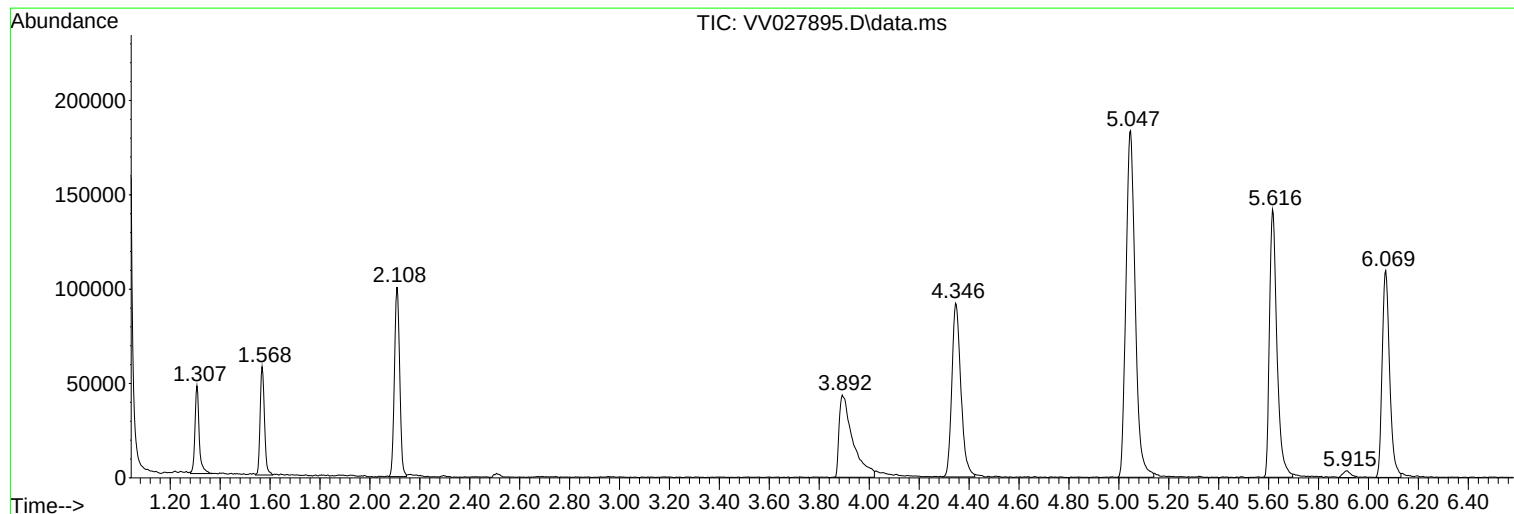

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027895.D
Acq On : 16 Sep 2022 20:53
Operator : SY/MD
Sample : N4672-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091622\
Data File : VV027895.D
Acq On : 16 Sep 2022 20:53
Operator : SY/MD
Sample : N4672-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc