

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
 Data File : VV039095.D
 Acq On : 16 Sep 2025 10:56
 Operator : SY/MD
 Sample : Q3084-06 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-6(20250910)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV039095.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.291	71	78	92	rBV	149369	188143	7.10%	1.261%
2	1.545	149	157	172	rBV	141969	198013	7.47%	1.327%
3	2.072	310	321	340	rBV	281215	491462	18.55%	3.295%
4	3.812	853	862	892	rBV	75481	270698	10.22%	1.815%
5	4.256	984	1000	1032	rBV2	208983	610049	23.02%	4.090%
6	4.960	1205	1219	1255	rBV2	448300	1297556	48.97%	8.699%
7	5.535	1384	1398	1431	rBV	346303	834901	31.51%	5.597%
8	5.989	1526	1539	1567	rBV	274861	637232	24.05%	4.272%
9	6.915	1818	1827	1856	rBV2	102707	235362	8.88%	1.578%
10	7.239	1918	1928	1963	rBV	456592	915788	34.56%	6.139%
11	7.558	2019	2027	2055	rBV2	61433	139901	5.28%	0.938%
12	8.018	2161	2170	2196	rBV2	365920	773075	29.17%	5.183%
13	8.780	2394	2407	2408	rBV	761198	860965	32.49%	5.772%
14	8.802	2409	2414	2444	rVB	1548740	2649819	100.00%	17.764%
15	10.143	2820	2831	2856	rBV	206130	342955	12.94%	2.299%
16	11.107	3121	3131	3143	rBV	360631	569203	21.48%	3.816%
17	11.197	3143	3159	3187	rVB2	940248	2322913	87.66%	15.573%
18	11.548	3257	3268	3294	rBV2	487108	930126	35.10%	6.235%
19	13.185	3764	3777	3799	rBV	387768	648498	24.47%	4.347%




Sum of corrected areas: 14916659

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
Data File : VV039095.D
Acq On : 16 Sep 2025 10:56
Operator : SY/MD
Sample : Q3084-06 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-6(20250910)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

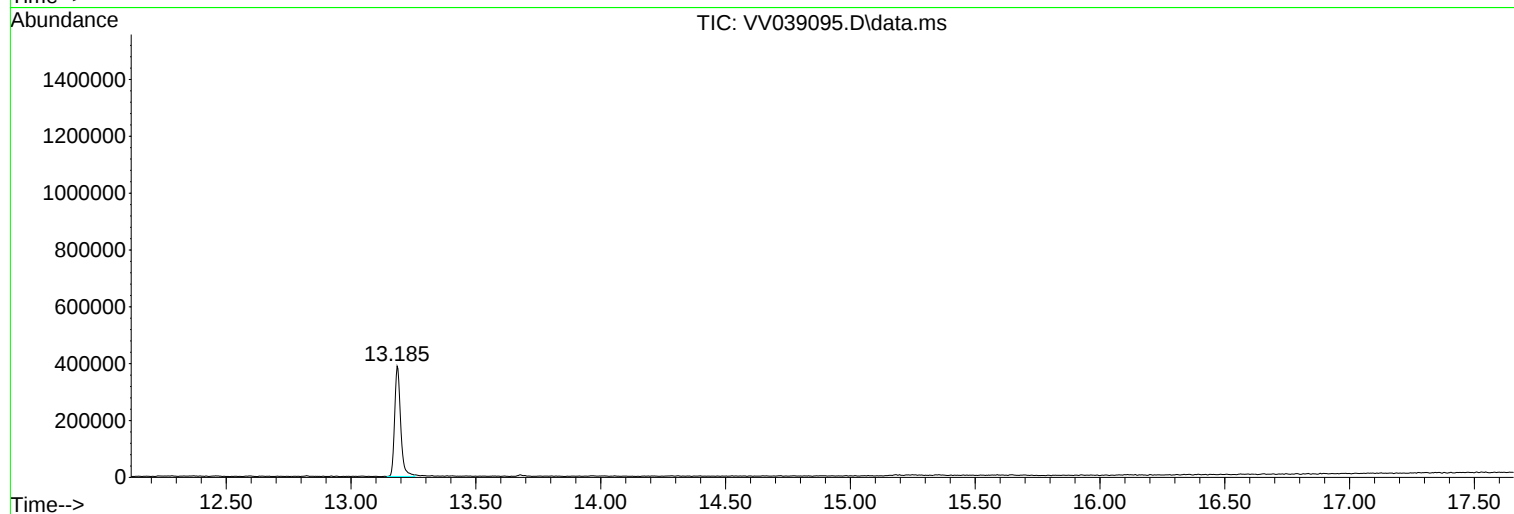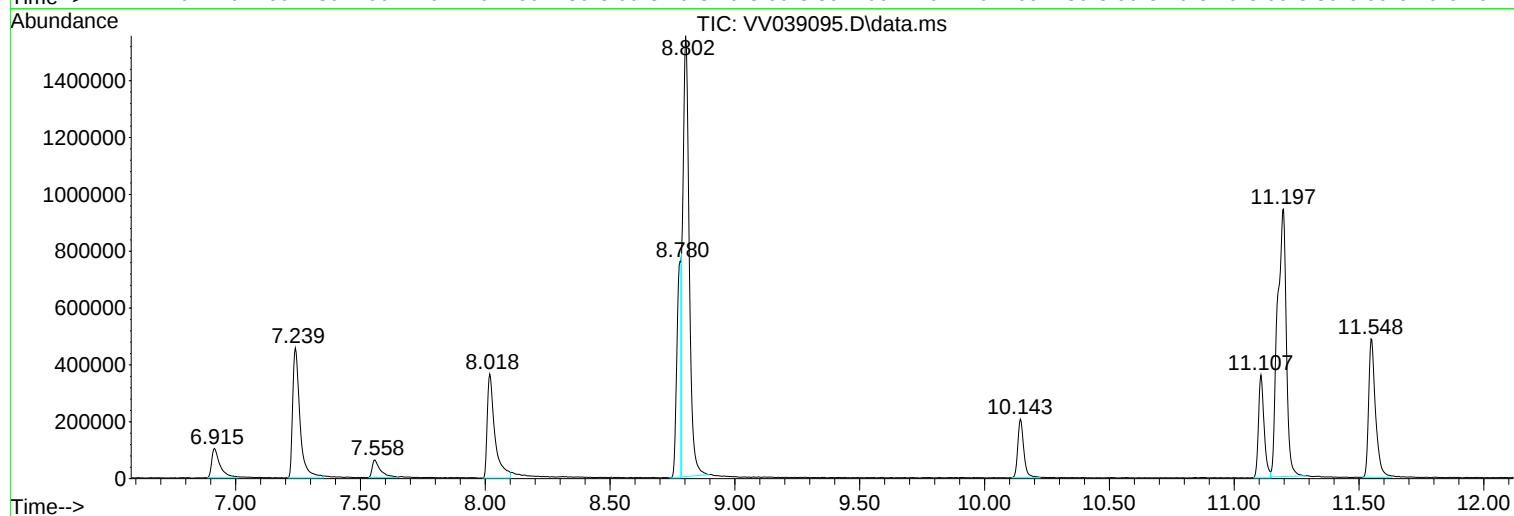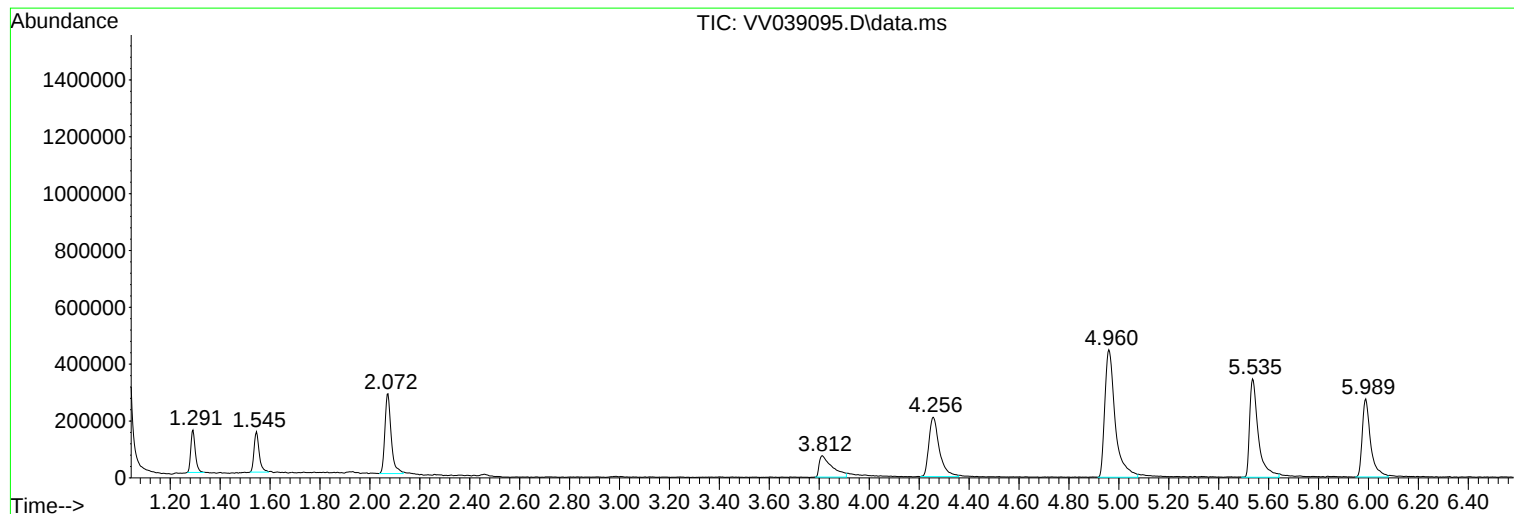

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
Data File : VV039095.D
Acq On : 16 Sep 2025 10:56
Operator : SY/MD
Sample : Q3084-06 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-6(20250910)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
Data File : VV039095.D
Acq On : 16 Sep 2025 10:56
Operator : SY/MD
Sample : Q3084-06 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-6(20250910)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc