

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
 Data File : VV039108.D
 Acq On : 16 Sep 2025 15:37
 Operator : SY/MD
 Sample : Q3084-02DL 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-9D(20250909)DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV039108.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.291	71	78	95	rVB	142161	182585	14.18%	1.569%
2	1.545	149	157	170	rBV	142161	203120	15.78%	1.746%
3	2.073	310	321	341	rBV	264213	470373	36.54%	4.043%
4	2.458	433	441	459	rBV2	21277	41526	3.23%	0.357%
5	3.796	849	857	894	rBV	99516	335095	26.03%	2.880%
6	4.256	984	1000	1030	rBV2	204695	601152	46.70%	5.167%
7	4.960	1200	1219	1259	rBV2	430768	1231294	95.65%	10.583%
8	5.535	1387	1398	1433	rBV	376210	913868	70.99%	7.855%
9	5.989	1526	1539	1569	rBV2	263850	617732	47.99%	5.309%
10	6.915	1816	1827	1850	rBV2	101993	229892	17.86%	1.976%
11	7.240	1918	1928	1956	rBV	438253	878192	68.22%	7.548%
12	7.558	2017	2027	2051	rBV3	58223	135602	10.53%	1.165%
13	8.018	2161	2170	2204	rBV	398773	839378	65.20%	7.214%
14	8.776	2396	2406	2441	rBV	699773	1287305	100.00%	11.064%
15	10.143	2818	2831	2850	rBV	201703	343055	26.65%	2.949%
16	11.114	3124	3133	3143	rBV3	62248	104209	8.10%	0.896%
17	11.175	3143	3152	3189	rVB2	591928	1249315	97.05%	10.738%
18	11.548	3257	3268	3289	rBV	418404	723969	56.24%	6.222%
19	13.185	3766	3777	3793	rBV	757952	1193372	92.70%	10.257%
20	13.673	3920	3929	3943	rBV3	31258	53751	4.18%	0.462%




Sum of corrected areas: 11634785

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
Data File : VV039108.D
Acq On : 16 Sep 2025 15:37
Operator : SY/MD
Sample : Q3084-02DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-9D(20250909)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

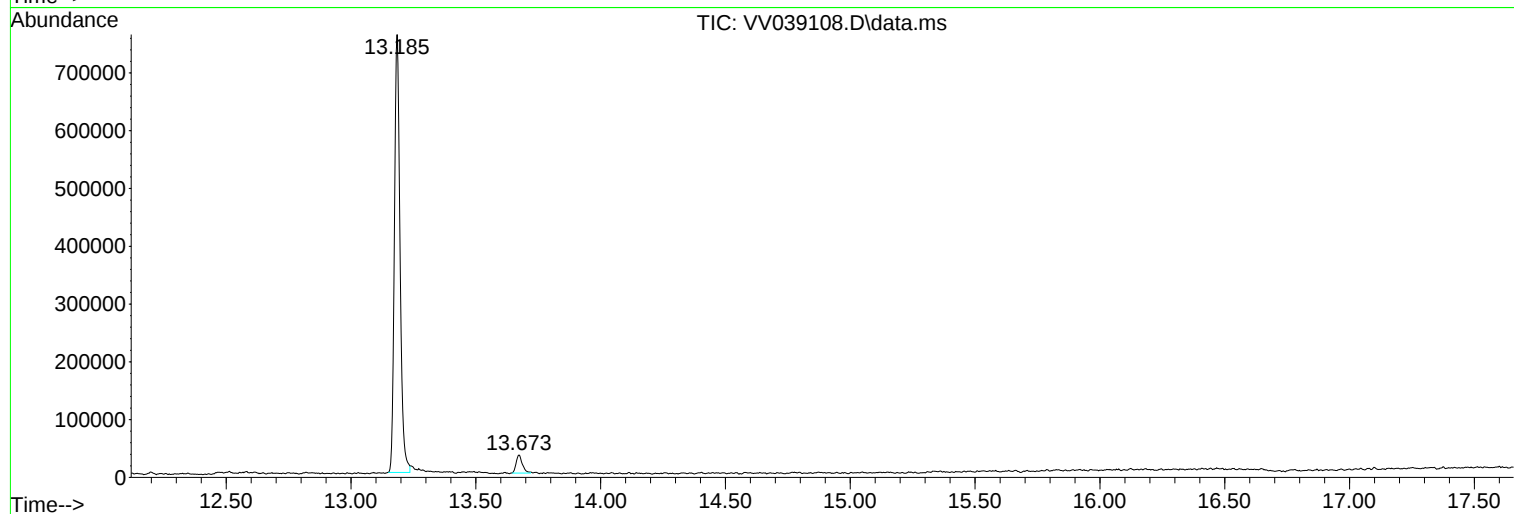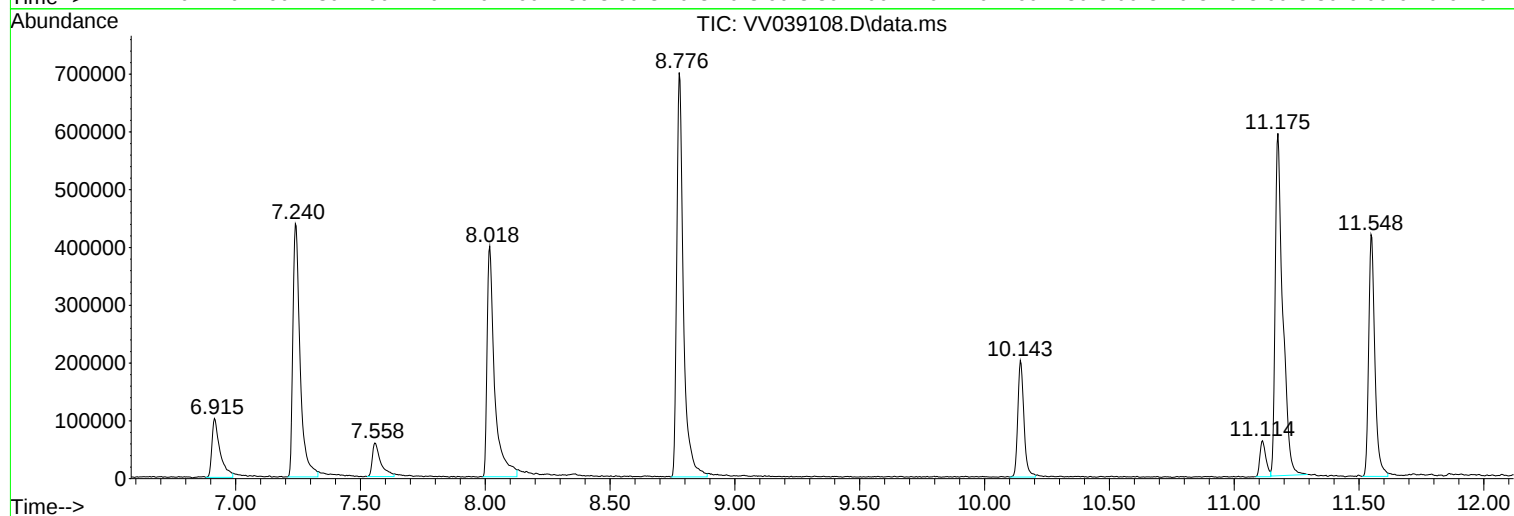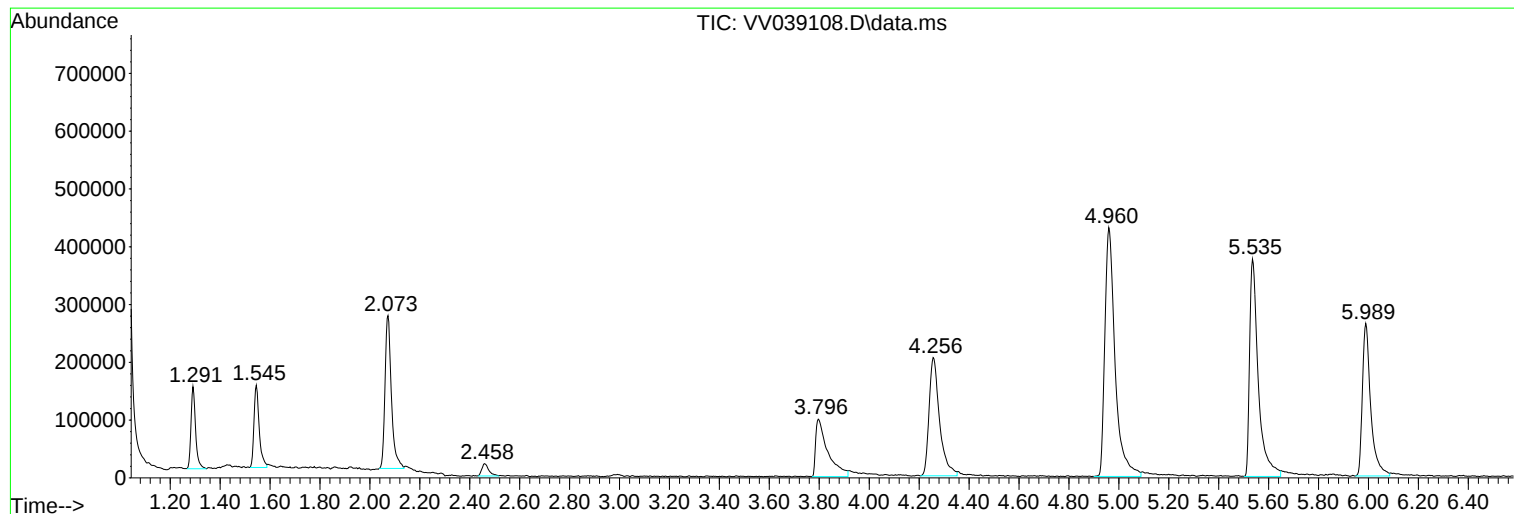

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
Data File : VV039108.D
Acq On : 16 Sep 2025 15:37
Operator : SY/MD
Sample : Q3084-02DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-9D(20250909)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
Data File : VV039108.D
Acq On : 16 Sep 2025 15:37
Operator : SY/MD
Sample : Q3084-02DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-9D(20250909)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc