

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
 Data File : VV039110.D
 Acq On : 16 Sep 2025 16:20
 Operator : SY/MD
 Sample : Q3084-08DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-7S(20250910)DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV039110.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.291	71	78	93	rBV	150180	192193	5.01%	1.315%
2	1.545	150	157	173	rVB	129106	189481	4.94%	1.297%
3	2.072	310	321	338	rBV	255031	454264	11.84%	3.109%
4	2.461	432	442	453	rBV	21472	39849	1.04%	0.273%
5	2.712	508	520	541	rBV3	27679	66427	1.73%	0.455%
6	3.124	636	648	669	rBV2	31089	78916	2.06%	0.540%
7	3.818	848	864	903	rBV4	194300	792963	20.66%	5.427%
8	4.256	983	1000	1034	rBV	204945	603560	15.73%	4.131%
9	4.960	1205	1219	1269	rBV2	443254	1301912	33.93%	8.910%
10	5.535	1388	1398	1430	rBV	407025	964193	25.12%	6.599%
11	5.989	1527	1539	1577	rBV2	267272	641973	16.73%	4.394%
12	6.915	1818	1827	1860	rBV	99812	233947	6.10%	1.601%
13	7.239	1919	1928	1959	rBV	448097	894890	23.32%	6.125%
14	7.558	2018	2027	2047	rBV	60789	133805	3.49%	0.916%
15	8.018	2161	2170	2204	rBV	410856	864900	22.54%	5.919%
16	8.776	2395	2406	2440	rBV2	748174	1657713	43.20%	11.345%
17	10.143	2819	2831	2850	rBV	203519	347440	9.05%	2.378%
18	11.107	3121	3131	3143	rBV	300971	496377	12.93%	3.397%
19	11.194	3143	3158	3190	rVB2	1820886	3837603	100.00%	26.265%
20	11.548	3257	3268	3291	rBV	463251	818946	21.34%	5.605%




Sum of corrected areas: 14611352

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
Data File : VV039110.D
Acq On : 16 Sep 2025 16:20
Operator : SY/MD
Sample : Q3084-08DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-7S(20250910)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

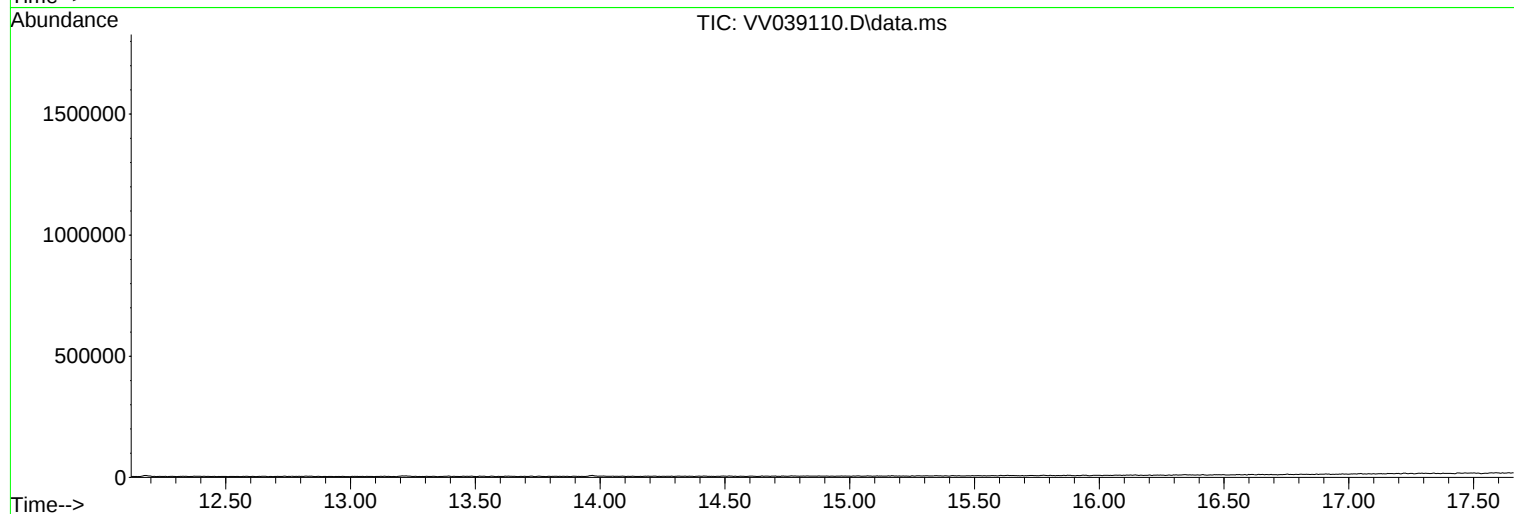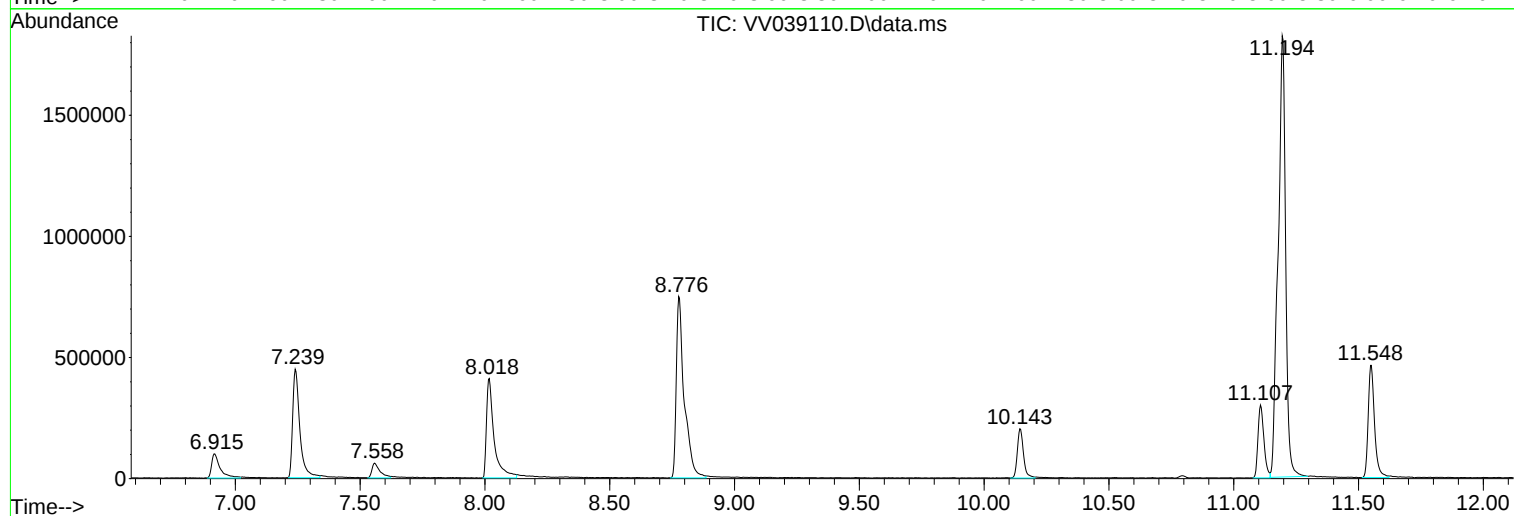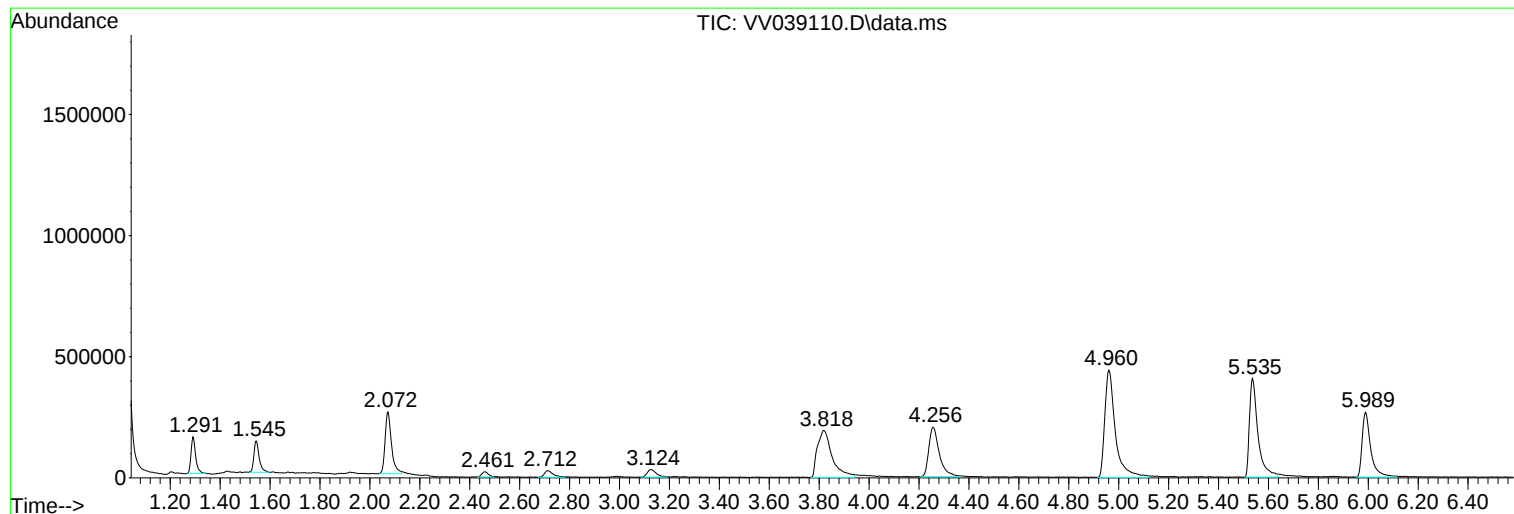

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
Data File : VV039110.D
Acq On : 16 Sep 2025 16:20
Operator : SY/MD
Sample : Q3084-08DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-7S(20250910)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
Data File : VV039110.D
Acq On : 16 Sep 2025 16:20
Operator : SY/MD
Sample : Q3084-08DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-7S(20250910)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc