

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
 Data File : VV039111.D
 Acq On : 16 Sep 2025 16:42
 Operator : SY/MD
 Sample : Q3084-09DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-7D(20250910)DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV039111.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.291	71	78	95	rVB	150749	195382	5.02%	1.347%
2	1.545	149	157	170	rBV	127978	183557	4.71%	1.265%
3	2.072	311	321	350	rVB	257306	468247	12.02%	3.228%
4	2.461	433	442	453	rBV2	22613	42910	1.10%	0.296%
5	2.709	511	519	535	rBV2	27515	60329	1.55%	0.416%
6	3.124	637	648	664	rBV2	29895	74621	1.92%	0.514%
7	3.818	848	864	893	rBV3	193628	756635	19.43%	5.216%
8	4.256	984	1000	1026	rBV2	206077	594169	15.25%	4.096%
9	4.960	1205	1219	1257	rBV2	426283	1267248	32.54%	8.736%
10	5.535	1388	1398	1429	rBV	396150	942299	24.19%	6.496%
11	5.989	1524	1539	1569	rBV	270197	628480	16.14%	4.332%
12	6.915	1818	1827	1859	rBV	97538	226695	5.82%	1.563%
13	7.239	1915	1928	1953	rBV	441931	874681	22.46%	6.030%
14	7.558	2016	2027	2052	rBV2	58252	134044	3.44%	0.924%
15	8.017	2159	2170	2206	rBV	401831	859842	22.08%	5.927%
16	8.776	2395	2406	2435	rBV2	739820	1632511	41.91%	11.254%
17	10.143	2822	2831	2852	rBV	196014	336325	8.63%	2.318%
18	11.107	3121	3131	3143	rBV	319763	515946	13.25%	3.557%
19	11.197	3143	3159	3189	rVB2	1873131	3894960	100.00%	26.849%
20	11.551	3258	3269	3298	rBV	459701	817775	21.00%	5.637%




Sum of corrected areas: 14506656

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
Data File : VV039111.D
Acq On : 16 Sep 2025 16:42
Operator : SY/MD
Sample : Q3084-09DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-7D(20250910)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

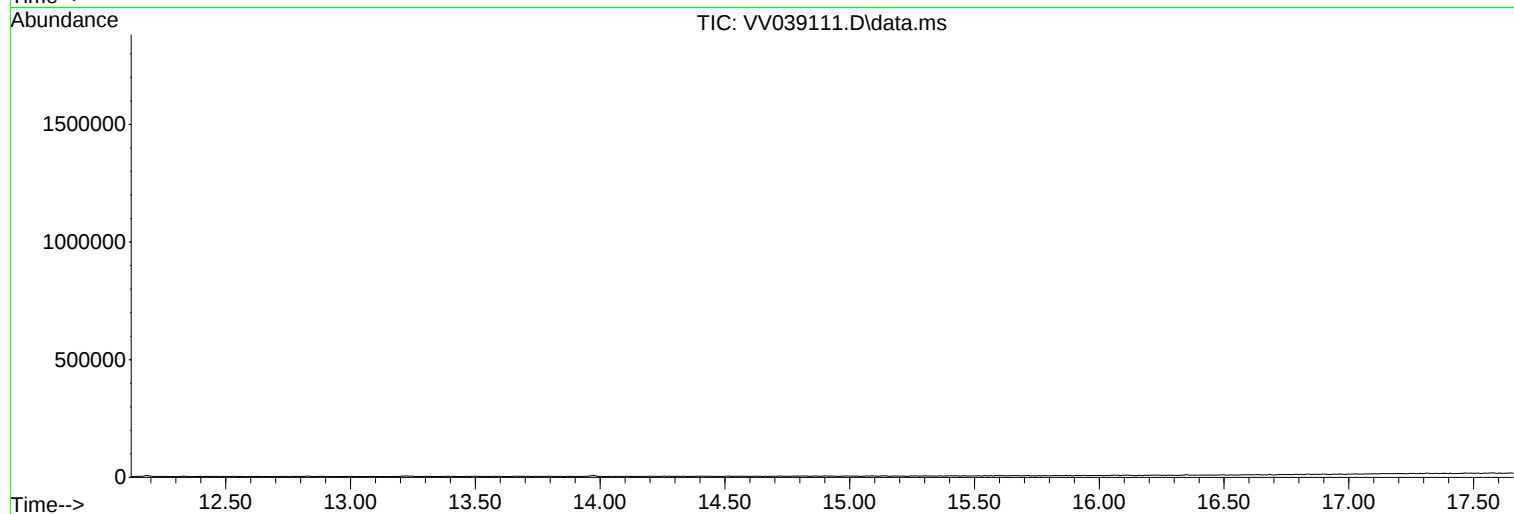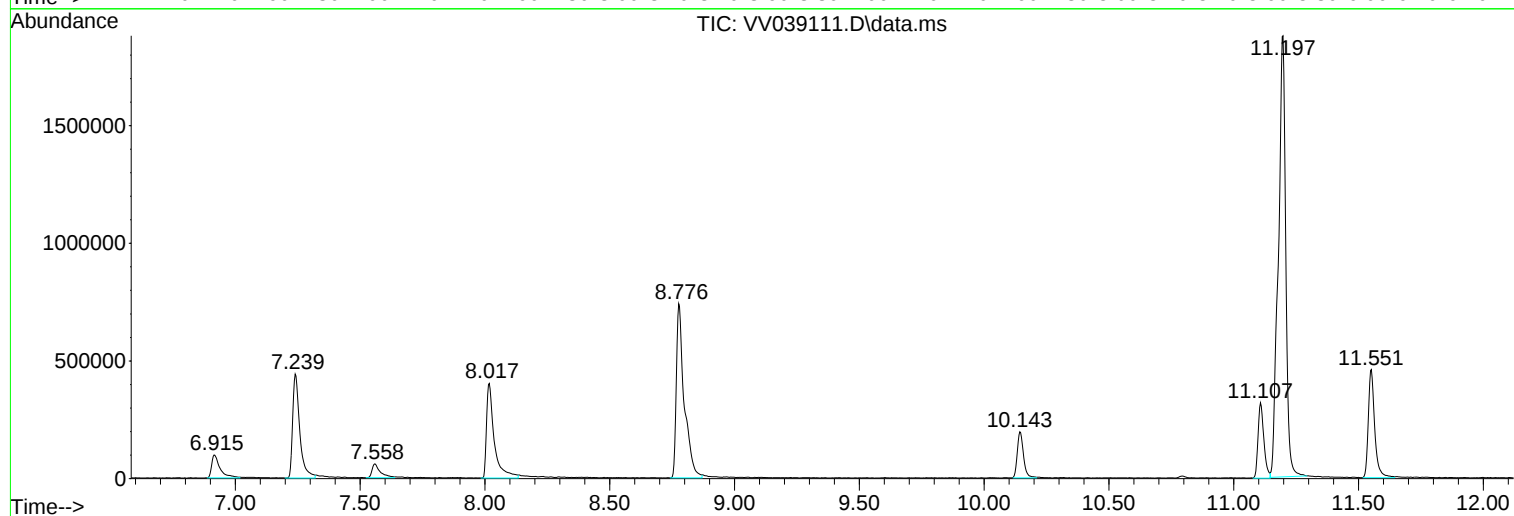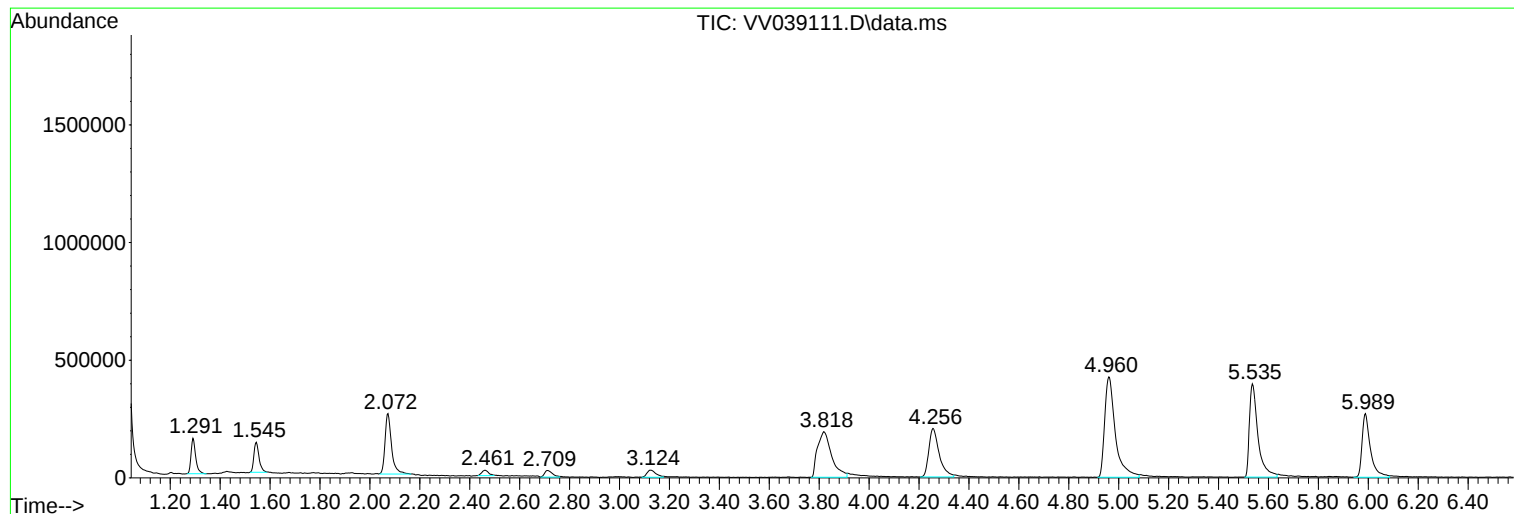

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
Data File : VV039111.D
Acq On : 16 Sep 2025 16:42
Operator : SY/MD
Sample : Q3084-09DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-7D(20250910)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
Data File : VV039111.D
Acq On : 16 Sep 2025 16:42
Operator : SY/MD
Sample : Q3084-09DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-7D(20250910)DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc