

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
 Data File : VV039114.D
 Acq On : 16 Sep 2025 17:46
 Operator : SY/MD
 Sample : VIBLK222
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK222

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV039114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.291	71	78	91	rBV	154600	196969	14.72%	1.896%
2	1.545	149	157	171	rBV	140802	201492	15.05%	1.939%
3	2.072	311	321	342	rVB	284945	490551	36.65%	4.721%
4	2.458	431	441	455	rBV3	25373	49247	3.68%	0.474%
5	3.796	846	857	896	rBV	112013	385718	28.82%	3.712%
6	4.256	984	1000	1029	rBV2	217113	643255	48.06%	6.191%
7	4.960	1201	1219	1262	rBV3	465476	1338551	100.00%	12.883%
8	5.538	1387	1399	1428	rBV2	354901	864875	64.61%	8.324%
9	5.989	1522	1539	1566	rBV3	283211	658373	49.19%	6.336%
10	6.915	1817	1827	1853	rBV	108469	241968	18.08%	2.329%
11	7.239	1918	1928	1971	rBV	482822	975711	72.89%	9.391%
12	7.558	2017	2027	2043	rBV2	63397	136399	10.19%	1.313%
13	8.017	2161	2170	2202	rBV	454414	934616	69.82%	8.995%
14	8.776	2396	2406	2442	rBV	628739	1151010	85.99%	11.078%
15	9.371	2586	2591	2598	rBV	21760	17369	1.30%	0.167%
16	10.143	2817	2831	2853	rBV	219824	377002	28.16%	3.628%
17	11.123	3127	3136	3142	rBV5	13260	21700	1.62%	0.209%
18	11.175	3142	3152	3182	rVV	522486	959465	71.68%	9.234%
19	11.551	3257	3269	3288	rBV	436017	746075	55.74%	7.180%




Sum of corrected areas: 10390346

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
Data File : VV039114.D
Acq On : 16 Sep 2025 17:46
Operator : SY/MD
Sample : VIBLK222
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK222

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

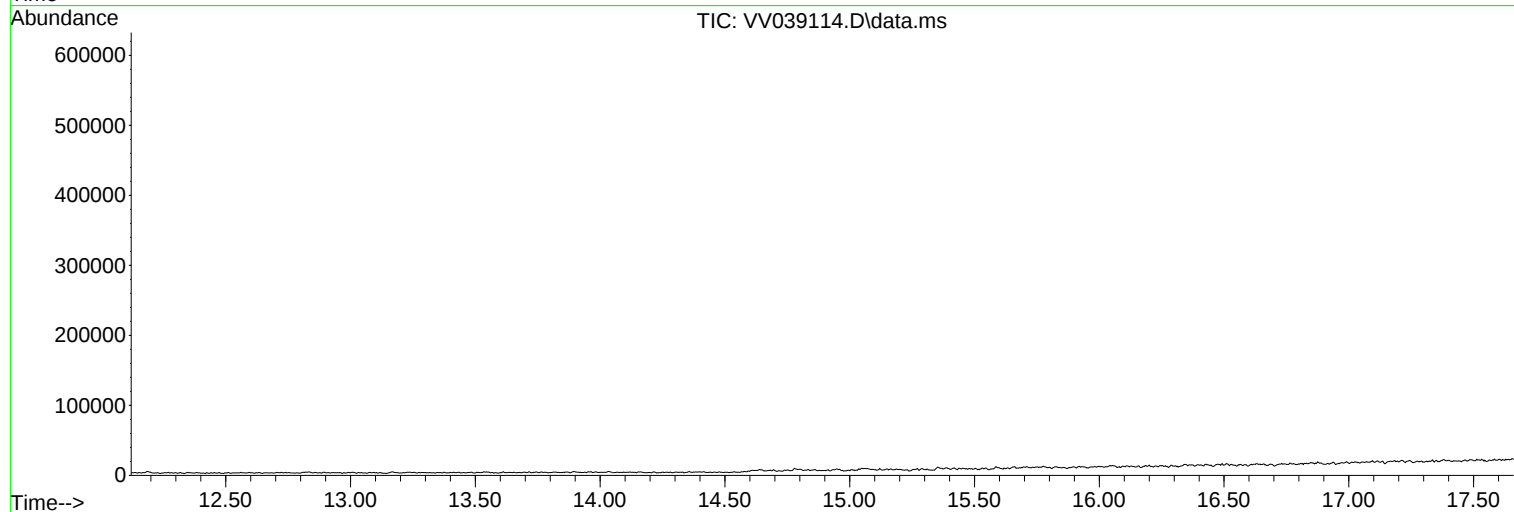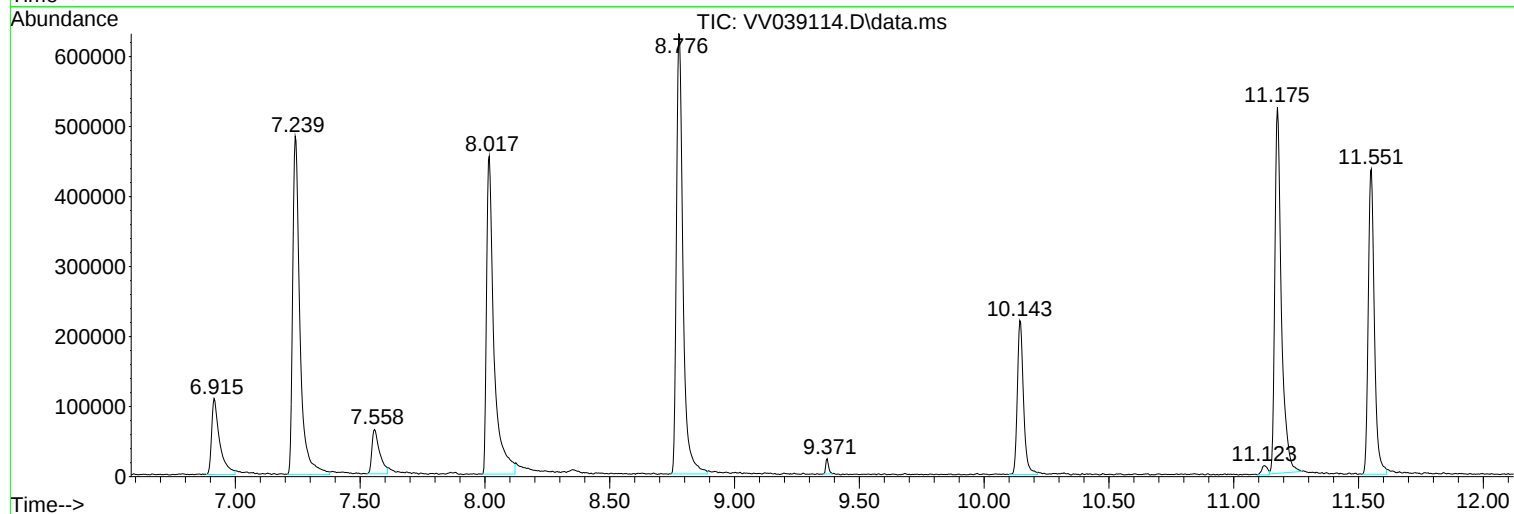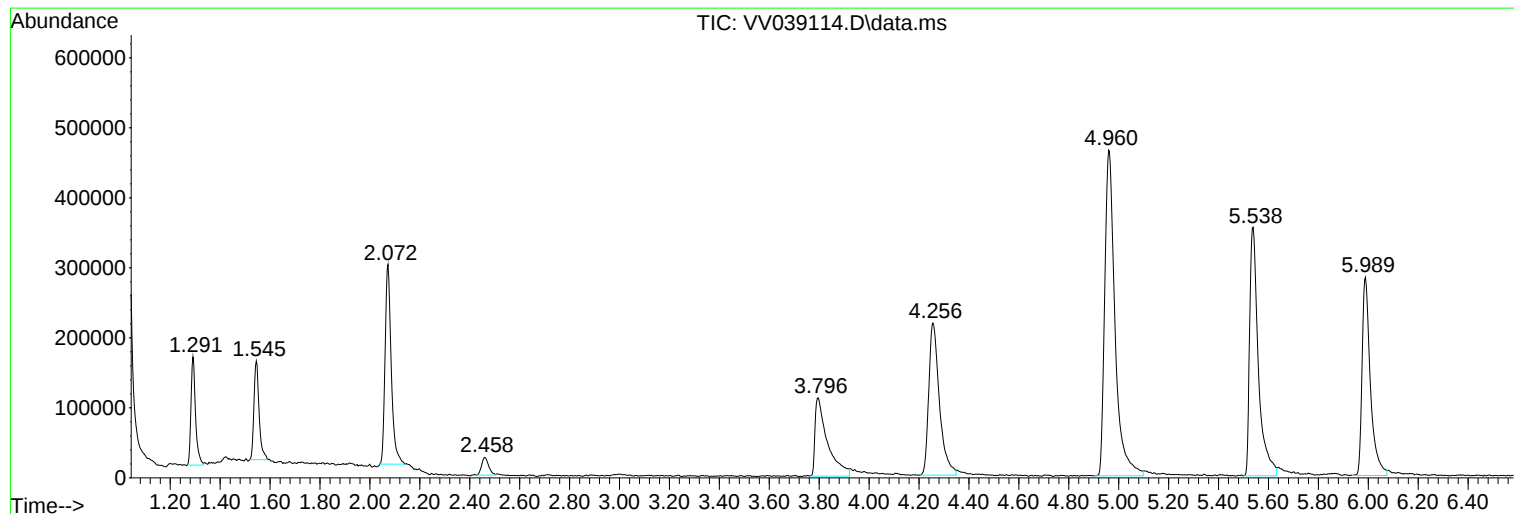

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
Data File : VV039114.D
Acq On : 16 Sep 2025 17:46
Operator : SY/MD
Sample : VIBLK222
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK222

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
Data File : VV039114.D
Acq On : 16 Sep 2025 17:46
Operator : SY/MD
Sample : VIBLK222
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK222

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc