
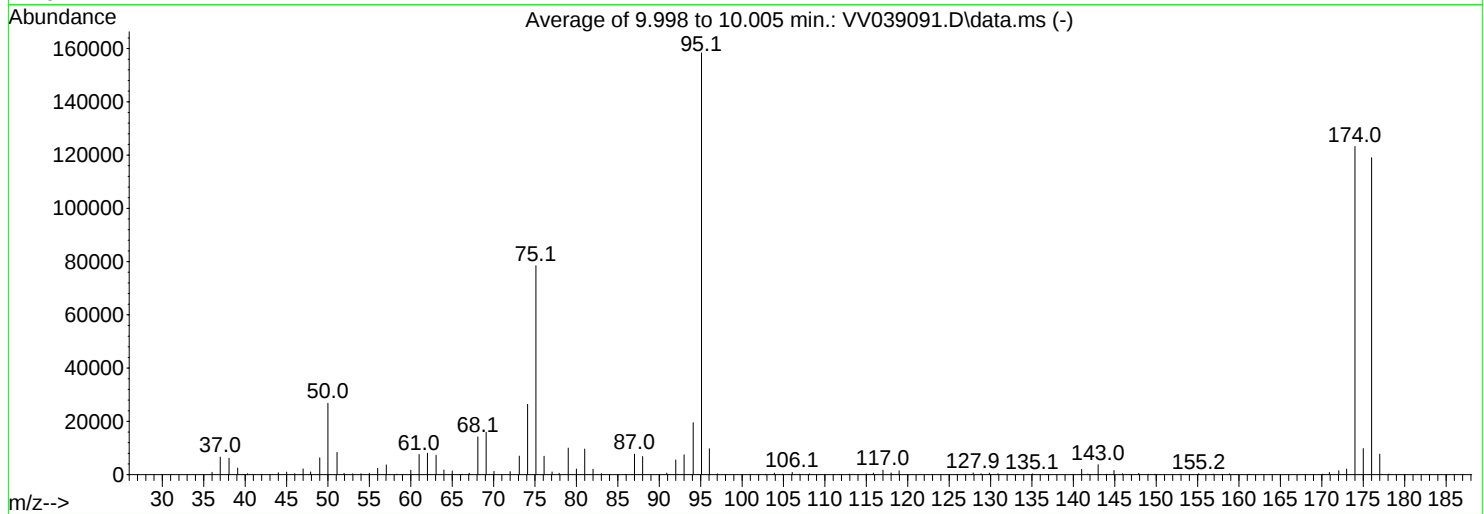


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091625\
Data File : VV039091.D
Acq On : 16 Sep 2025 08:58
Operator : SY/MD
Sample : BFB211
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB211

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Sep 17 02:19:46 2025

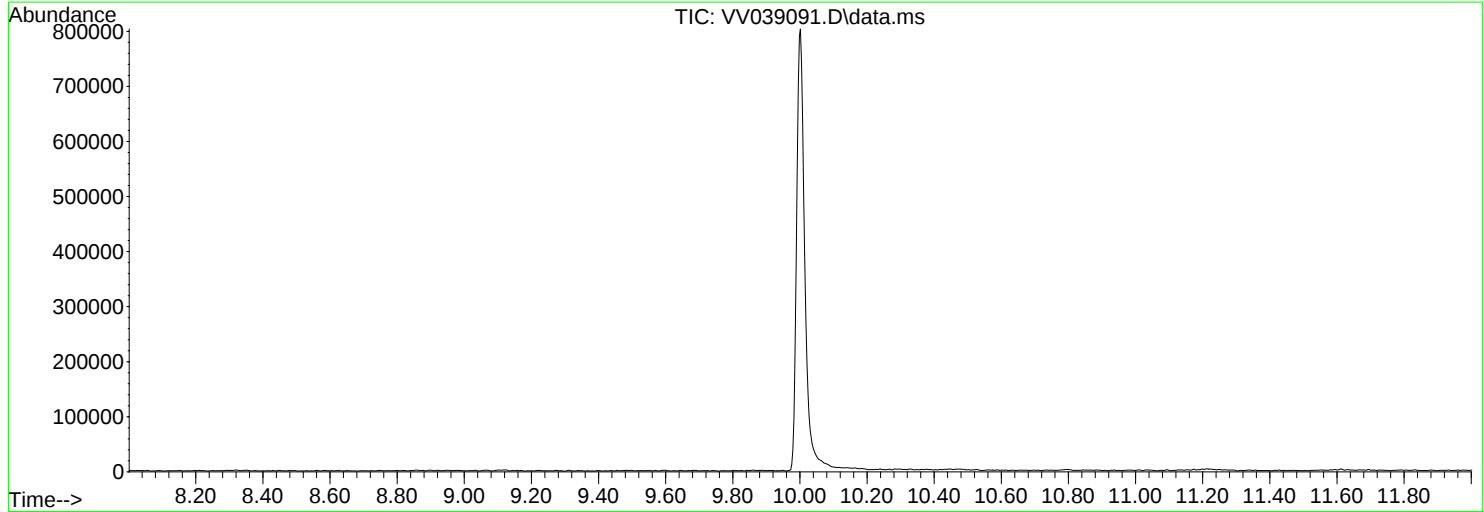

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2774

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	26805	PASS
75	95	30	80	49.6	78488	PASS
95	95	100	100	100.0	158400	PASS
96	95	5	9	6.2	9751	PASS
173	174	0.00	2	1.7	2133	PASS
174	95	50	120	77.8	123227	PASS
175	174	5	9	7.9	9778	PASS
176	174	95	105	96.6	119053	PASS
177	176	5	10	6.5	7701	PASS

m/z	Abundance
39.90	526.0
42.30	120.0
43.90	694.0
44.90	146.0
62.10	103.0
77.10	124.0
99.50	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
36.00	1098.0
37.00	6695.0
38.10	6407.0
39.10	2504.0
39.90	704.0
44.10	1512.0
45.10	988.0
46.00	325.0
47.00	2317.0
47.90	1088.0
49.00	6428.0
50.00	28080.0
51.10	8762.0
52.00	472.0
52.90	333.0
54.00	372.0
55.00	518.0
56.00	2477.0
57.00	3710.0
58.20	189.0
60.00	1767.0
61.00	7717.0
62.00	8511.0
63.00	7558.0
64.00	2020.0
65.00	1170.0
66.20	232.0
67.00	508.0
68.10	14670.0
69.10	16326.0
70.10	1094.0
72.00	1224.0
73.10	7297.0
74.10	27184.0
75.10	80840.0
76.10	7393.0
77.00	1305.0
77.90	698.0
79.00	9968.0
80.00	2132.0
81.00	9628.0
82.00	2065.0
83.00	336.0
87.00	7704.0
88.00	6640.0
90.90	684.0
92.00	5529.0
93.00	7309.0
94.10	20360.0
95.10	161920.0
96.00	9833.0
97.00	305.0
102.80	196.0
103.80	696.0
104.90	225.0
106.00	871.0
106.90	189.0
108.10	344.0
110.00	142.0
111.00	177.0
113.00	230.0
115.00	221.0
115.90	619.0
117.00	1682.0
118.00	779.0
119.00	1612.0
127.90	576.0
128.90	425.0
129.90	723.0
130.90	341.0
133.30	126.0
135.00	264.0
136.70	208.0
137.00	210.0
141.00	2056.0
141.80	231.0
143.00	4082.0
143.90	212.0
144.90	1577.0
145.90	302.0
146.80	134.0
147.90	430.0
149.10	238.0
149.80	123.0
152.90	163.0
154.00	172.0
155.10	376.0
157.00	221.0
158.90	299.0
161.20	180.0
170.10	140.0
170.90	809.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

172.00	1278.0
173.00	2295.0
174.00	123816.0
175.00	10047.0
176.00	117536.0
177.00	7521.0
178.00	292.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
36.00	946.0
37.00	6876.0
38.10	6346.0
39.10	2505.0
39.90	687.0
40.30	568.0
41.90	105.0
44.00	1370.0
45.00	1111.0
46.00	379.0
47.00	2289.0
47.90	1062.0
49.00	6580.0
50.00	27488.0
51.10	8490.0
51.90	543.0
53.00	345.0
54.00	393.0
55.00	578.0
56.00	2372.0
57.10	3699.0
58.30	144.0
60.00	1755.0
61.00	7894.0
62.00	8500.0
63.10	7314.0
64.00	1791.0
65.00	1472.0
66.20	207.0
67.00	604.0
68.10	14524.0
69.10	16504.0
70.00	1361.0
72.00	1172.0
73.10	7153.0
74.10	27032.0
75.10	80800.0
76.10	7109.0
77.10	1196.0
77.90	509.0
79.00	10380.0
80.00	2198.0
81.00	9851.0
82.00	2131.0
83.00	370.0
85.90	169.0
87.00	7946.0
88.00	7029.0
90.90	677.0
92.00	5766.0
93.00	7760.0
94.10	20360.0
95.10	162688.0
96.10	10034.0
97.00	337.0
102.80	211.0
103.90	631.0
104.90	195.0
106.10	878.0
106.90	181.0
108.10	341.0
109.90	141.0
111.20	165.0
111.80	136.0
112.90	247.0
115.00	287.0
115.80	630.0
117.00	1688.0
118.00	732.0
118.90	1499.0
127.90	733.0
128.90	383.0
129.80	606.0
130.90	417.0
135.10	302.0
136.80	201.0
141.00	2065.0
141.70	256.0
143.00	3934.0
143.90	178.0
144.90	1562.0
146.00	373.0
146.90	117.0
147.90	463.0
149.10	210.0
149.80	168.0
152.90	233.0
154.00	154.0
155.10	330.0
157.00	213.0
158.90	313.0
161.20	185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

170.00	194.0
170.90	877.0
172.10	1560.0
173.00	2233.0
174.00	127376.0
175.00	9976.0
176.00	122776.0
177.00	8057.0
178.10	278.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
36.00	749.0
37.00	6252.0
38.00	5800.0
39.10	2409.0
39.90	560.0
40.30	546.0
41.90	132.0
44.00	1319.0
45.00	1179.0
46.00	371.0
47.00	1971.0
47.90	889.0
49.00	5894.0
50.00	24848.0
51.10	7754.0
51.90	639.0
53.00	313.0
54.00	363.0
55.00	571.0
56.00	2189.0
57.10	3630.0
58.40	191.0
60.00	1531.0
61.00	7207.0
62.00	7542.0
63.10	6940.0
64.00	1467.0
65.00	1574.0
65.90	180.0
67.10	529.0
68.10	13387.0
69.10	14915.0
70.00	1369.0
72.00	980.0
73.10	6384.0
74.10	24960.0
75.10	73824.0
76.10	6255.0
77.10	944.0
77.90	378.0
79.00	9608.0
80.00	2042.0
81.00	9431.0
82.00	1951.0
83.00	333.0
85.90	281.0
87.00	7369.0
88.00	6668.0
90.90	530.0
92.00	5256.0
93.00	7252.0
94.10	17856.0
95.10	150592.0
96.10	9387.0
97.10	343.0
102.80	142.0
104.00	514.0
105.00	125.0
106.10	815.0
106.90	150.0
108.20	274.0
109.90	150.0
111.00	138.0
111.80	165.0
112.90	204.0
115.00	308.0
115.80	627.0
117.00	1610.0
118.00	572.0
118.90	1272.0
126.80	113.0
127.90	768.0
128.80	360.0
129.90	481.0
130.90	330.0
135.10	355.0
136.90	224.0
141.00	1808.0
141.70	225.0
143.00	3183.0
144.00	153.0
144.90	1603.0
146.00	355.0
146.90	100.0
147.90	553.0
149.00	162.0
149.90	210.0
152.90	229.0
154.10	122.0
155.20	327.0
156.90	272.0
158.80	283.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

161.20	118.0
170.00	152.0
170.90	853.0
172.10	1631.0
173.00	1871.0
174.00	118488.0
175.00	9310.0
176.00	116848.0
177.00	7526.0
178.20	185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211