


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091718\
 Data File : VV007580.D
 Acq On : 17 Sep 2018 09:21
 Operator : SY/MD
 Sample : BFB74
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB74

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091318WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Sep 18 03:38:22 2018

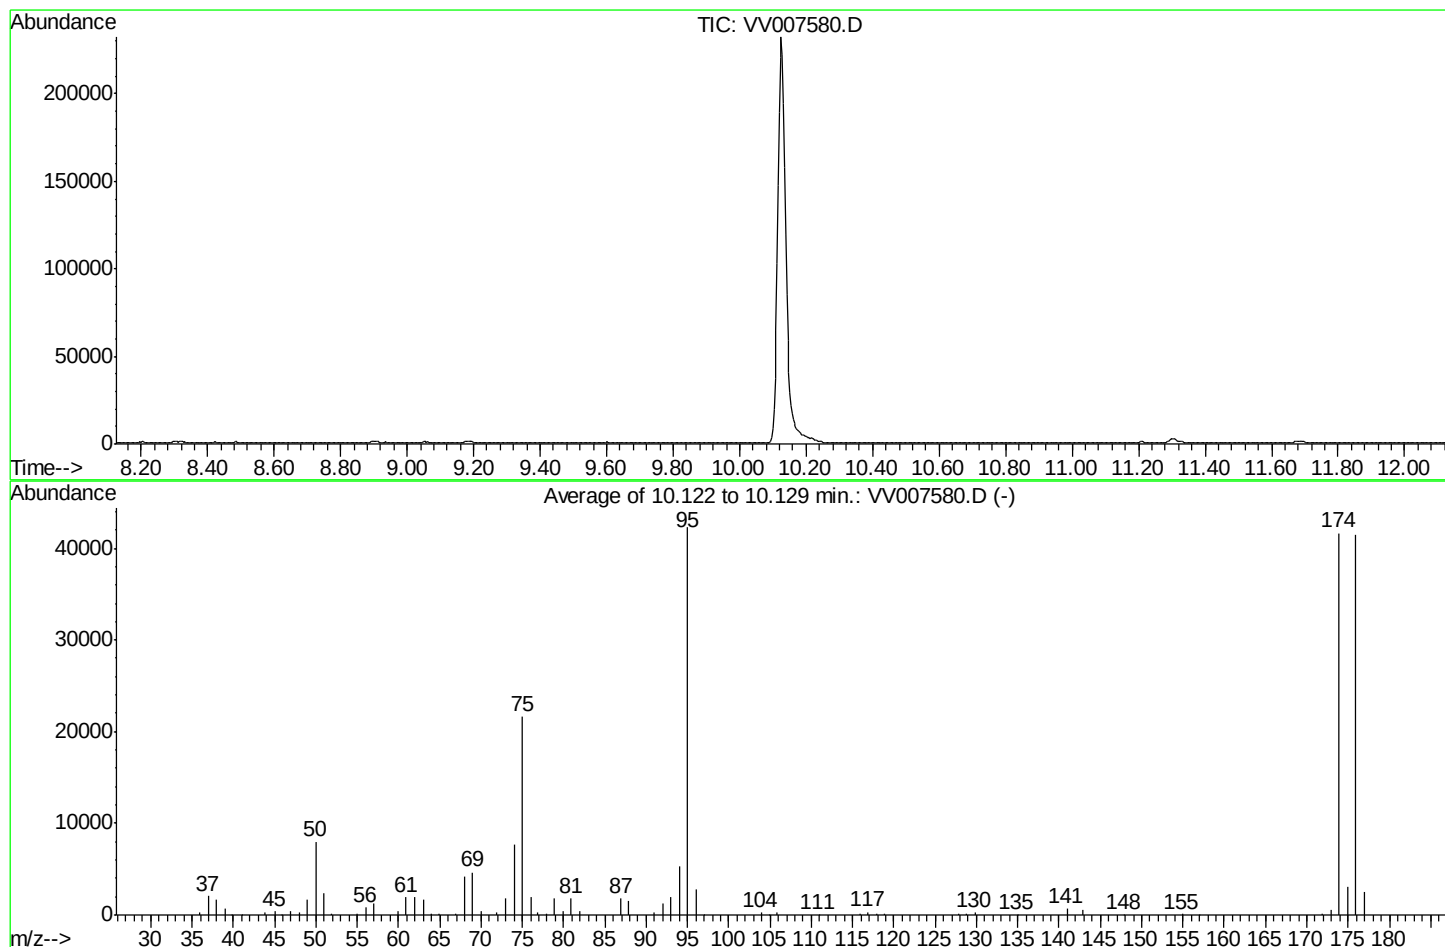

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	8013	PASS
75	95	30	80	51.0	21581	PASS
95	95	100	100	100.0	42285	PASS
96	95	5	9	6.5	2734	PASS
173	174	0.00	2	1.2	510	PASS
174	95	50	120	98.4	41626	PASS
175	174	5	9	7.3	3037	PASS
176	174	95	101	99.7	41514	PASS
177	176	5	9	6.1	2528	PASS

Scan 2797 (10.084 min): VV007580.D
BFB74

m/z	Abundance
39.80	186.0
42.90	114.0
44.00	270.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
35.90	361.0
37.00	2107.0
38.00	1709.0
38.90	767.0
39.90	277.0
41.00	118.0
42.90	124.0
43.90	576.0
45.00	389.0
46.90	453.0
47.90	289.0
49.00	1674.0
50.00	7952.0
51.00	2363.0
51.90	127.0
55.00	160.0
56.00	766.0
57.00	1281.0
59.90	400.0
60.90	1846.0
62.00	1888.0
63.00	1618.0
64.00	170.0
64.90	112.0
67.00	145.0
68.00	4267.0
69.00	4606.0
70.00	369.0
72.00	237.0
73.00	1713.0
74.00	7638.0
75.00	21448.0
76.00	1986.0
76.90	246.0
77.90	153.0
78.90	1774.0
79.90	469.0
80.90	1778.0
81.90	407.0
86.90	1595.0
87.90	1460.0
90.90	258.0
92.00	1278.0
92.90	2015.0
94.00	5185.0
95.00	41784.0
96.00	2763.0
103.90	248.0
105.80	201.0
115.80	219.0
116.80	340.0
117.90	200.0
118.80	230.0
127.80	132.0
128.80	102.0
129.80	208.0
134.90	102.0
140.90	613.0
142.90	580.0
147.80	118.0
155.00	107.0
171.80	175.0
173.00	496.0
173.90	40112.0
174.90	2930.0
175.90	39984.0
176.90	2539.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
35.90	354.0
37.00	2131.0
38.00	1668.0
39.00	766.0
39.90	259.0
42.90	109.0
43.90	577.0
45.00	448.0
45.90	101.0
46.90	482.0
48.00	291.0
49.00	1739.0
50.00	8252.0
51.00	2368.0
51.90	176.0
55.00	157.0
56.00	797.0
57.00	1309.0
60.00	410.0
61.00	2002.0
62.00	1946.0
63.00	1758.0
63.90	164.0
64.90	124.0
66.90	157.0
68.00	4368.0
69.00	4788.0
70.00	412.0
72.00	256.0
73.00	1804.0
74.00	7787.0
75.00	22208.0
76.00	2007.0
76.90	202.0
77.90	195.0
78.90	1892.0
79.90	457.0
80.90	1868.0
81.90	395.0
86.90	1817.0
87.90	1558.0
90.90	288.0
92.00	1294.0
93.00	2071.0
94.00	5432.0
95.00	43752.0
96.00	2818.0
97.00	108.0
103.90	261.0
104.90	101.0
105.90	227.0
110.90	111.0
115.80	206.0
116.80	344.0
117.80	199.0
118.80	198.0
127.90	157.0
128.80	113.0
129.80	225.0
134.90	111.0
140.90	681.0
142.90	622.0
147.90	107.0
154.90	127.0
171.90	192.0
173.00	519.0
173.90	42936.0
174.90	3184.0
175.90	42944.0
176.90	2588.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
35.90	320.0
37.00	1985.0
38.00	1555.0
39.00	688.0
39.90	244.0
42.90	105.0
43.90	554.0
45.00	416.0
45.90	101.0
46.90	454.0
48.00	263.0
49.00	1689.0
50.00	7837.0
51.00	2310.0
51.90	192.0
54.90	166.0
56.00	794.0
57.00	1272.0
60.00	365.0
61.00	1994.0
62.00	1916.0
63.00	1700.0
63.90	140.0
64.90	107.0
66.90	162.0
68.00	4060.0
69.00	4434.0
69.90	448.0
71.90	231.0
73.00	1826.0
74.00	7456.0
75.00	21088.0
76.00	1825.0
76.90	205.0
77.90	211.0
78.90	1757.0
79.90	437.0
80.90	1746.0
81.90	357.0
87.00	1840.0
87.90	1497.0
90.90	276.0
92.00	1278.0
93.00	1935.0
94.00	5132.0
95.00	41320.0
96.00	2623.0
97.00	108.0
103.90	245.0
105.90	235.0
110.90	112.0
115.90	188.0
116.90	321.0
117.80	197.0
118.80	197.0
127.90	162.0
128.80	103.0
129.80	229.0
141.00	629.0
142.90	589.0
154.80	159.0
157.00	102.0
171.90	186.0
173.00	516.0
173.90	41832.0
174.90	2997.0
175.90	41616.0
176.90	2457.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74