

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091720\
 Data File : VV018272.D
 Acq On : 17 Sep 2020 12:43
 Operator : SY/MD
 Sample : L4012-15RE
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWT3RE

Quant Time: Sep 18 06:45:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 18 06:17:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	201769	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	199735	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	97994	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	96726	58.82	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	117.64%
7) Chloroethane-d5	1.58	69	80368	59.73	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	119.46%
11) 1,1-Dichloroethene-d2	2.12	63	141063	46.77	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.54%
21) 2-Butanone-d5	3.91	46	124866	124.06	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	124.06%
24) Chloroform-d	4.38	84	176044	61.71	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	123.42%
26) 1,2-Dichloroethane-d4	5.06	65	116783	63.86	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	127.72%#
32) Benzene-d6	5.08	84	353091	61.75	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	123.50%
36) 1,2-Dichloropropane-d6	6.09	67	113851	62.67	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	125.34%#
41) Toluene-d8	7.34	98	313526	60.17	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	120.34%#
43) trans-1,3-Dichloropropene-	7.64	79	56361	61.05	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	122.10%
47) 2-Hexanone-d5	8.11	63	90784	131.92	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	131.92%#
57) 1,1,2,2-Tetrachloroethane-	10.24	84	150001	65.78	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	131.56%#
64) 1,2-Dichlorobenzene-d4	11.65	152	134558	66.86	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	133.72%#


Target Compounds					Ovalue
13) Acetone	2.20	43	4600	5.708 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091720\
Data File : VV018272.D
Acq On : 17 Sep 2020 12:43
Operator : SY/MD
Sample : L4012-15RE
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWT3RE

Quant Time: Sep 18 06:45:58 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 18 06:17:41 2020
Response via : Initial Calibration

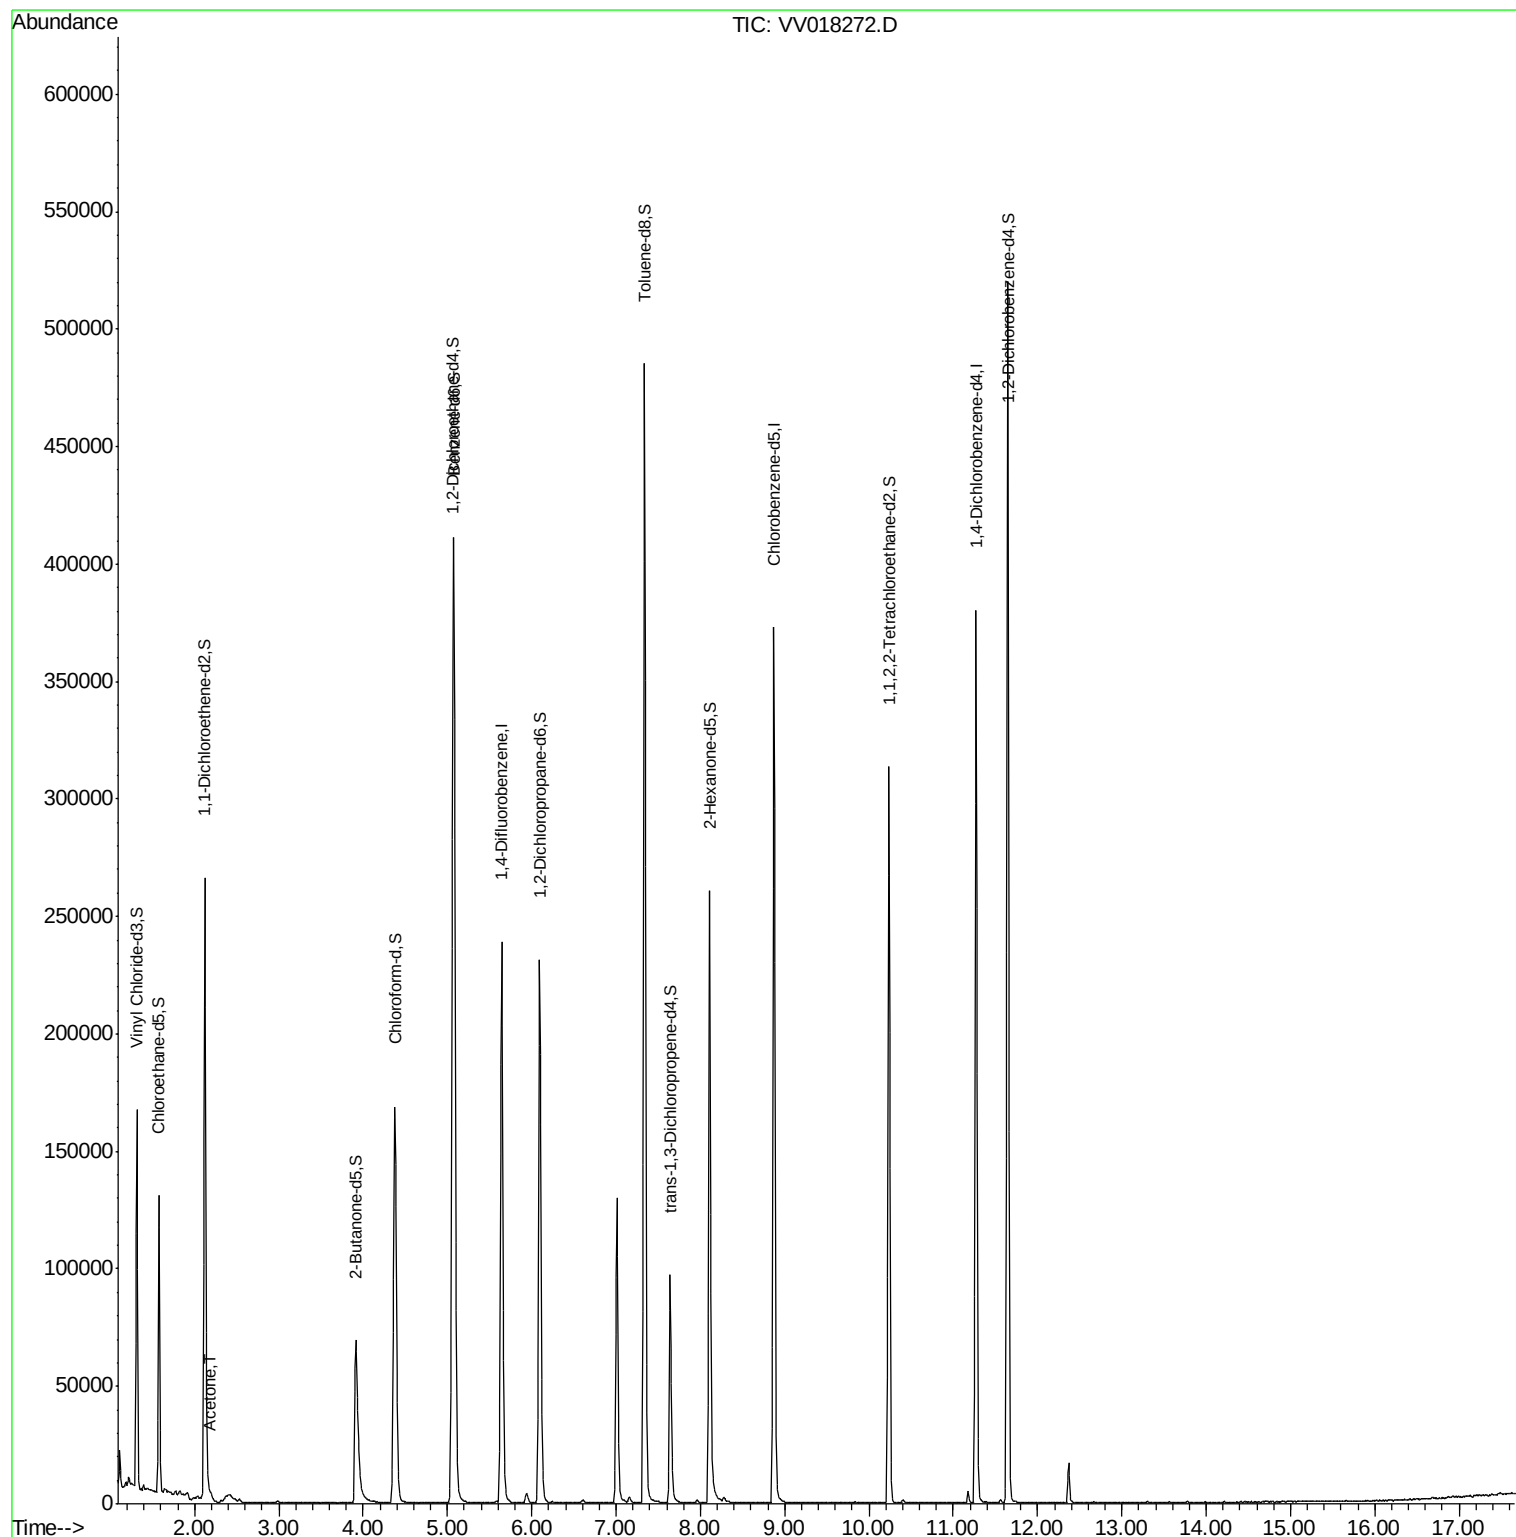

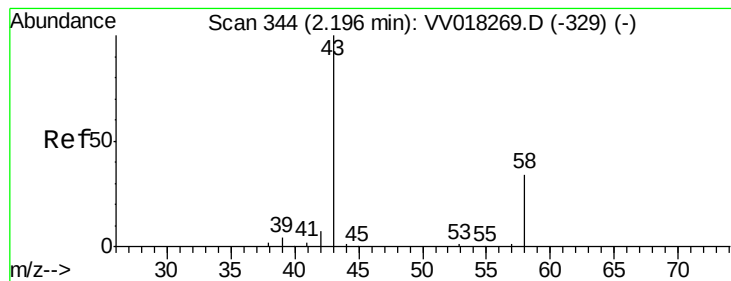

#13
 Acetone
 Concen: 5.708 ug/L
 RT: 2.20 min Scan# 344
 Delta R.T. 0.00 min
 Lab File: VV018272.D
 Acq: 17 Sep 2020 12:43

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWT3RE

Tot Ion: 43 Resp: 4600
 Ion Ratio Lower Upper
 43 100
 58 28.0 0.0 67.4

