

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091720\
 Data File : VV018272.D
 Acq On : 17 Sep 2020 12:43
 Operator : SY/MD
 Sample : L4012-15RE
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWT3RE

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	161806	166676	15.90%	2.213%
2	1.579	145	152	163	rVB	126211	142130	13.55%	1.887%
3	2.122	311	321	342	rBV	263467	391714	37.36%	5.200%
4	2.682	492	495	497	rBV	134	94	0.01%	0.001%
5	2.984	580	589	597	rVB4	948	1617	0.15%	0.021%
6	3.016	597	599	602	rBV2	185	78	0.01%	0.001%
7	3.039	604	606	607	rVB	108	24	0.00%	0.000%
8	3.065	611	614	616	rBV2	335	244	0.02%	0.003%
9	3.248	668	671	674	rBV	94	51	0.00%	0.001%
10	3.264	674	676	678	rVB	71	30	0.00%	0.000%
11	3.364	704	707	710	rBV	113	77	0.01%	0.001%
12	3.450	732	734	737	rBV	85	55	0.01%	0.001%
13	3.502	745	750	752	rBV	158	148	0.01%	0.002%
14	3.675	801	804	808	rVB2	142	120	0.01%	0.002%
15	3.695	808	810	812	rBV	34	14	0.00%	0.000%
16	3.714	812	816	818	rBV2	129	105	0.01%	0.001%
17	3.794	837	841	845	rBV2	88	74	0.01%	0.001%
18	3.820	845	849	852	rBV	147	93	0.01%	0.001%
19	3.872	863	865	867	rBV2	159	67	0.01%	0.001%
20	3.913	867	878	916	rBV	69215	202760	19.34%	2.692%
21	4.376	1005	1022	1053	rBV	168494	411303	39.23%	5.460%
22	4.566	1077	1081	1085	rBV3	281	288	0.03%	0.004%
23	4.608	1090	1094	1096	rBV2	162	130	0.01%	0.002%
24	4.650	1104	1107	1110	rVB	253	163	0.02%	0.002%
25	4.672	1110	1114	1119	rBV2	118	141	0.01%	0.002%
26	4.737	1132	1134	1137	rVB2	205	75	0.01%	0.001%
27	4.817	1156	1159	1162	rBV	106	73	0.01%	0.001%
28	4.843	1165	1167	1169	rBV2	45	23	0.00%	0.000%
29	4.872	1174	1176	1177	rBV	70	31	0.00%	0.000%
30	4.884	1177	1180	1183	rVV	132	83	0.01%	0.001%
31	4.904	1183	1186	1189	rVB2	92	61	0.01%	0.001%
32	5.016	1217	1221	1222	rBV	112	74	0.01%	0.001%
33	5.074	1222	1239	1268	rBV2	410989	1048545	100.00%	13.921%
34	5.376	1330	1333	1337	rBV2	247	215	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091720\
 Data File : VV018272.D
 Acq On : 17 Sep 2020 12:43
 Operator : SY/MD
 Sample : L4012-15RE
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWT3RE

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

35	5.470	1356	1362	1363	rBV2	99	96	0.01%	0.001%
36	5.582	1384	1397	1400	rBV3	669	1227	0.12%	0.016%
37	5.643	1404	1416	1444	rVV	238552	471119	44.93%	6.255%
38	5.942	1498	1509	1523	rVB6	4287	9345	0.89%	0.124%
39	6.093	1543	1556	1591	rBV	230916	470921	44.91%	6.252%
40	6.605	1706	1715	1727	rBV4	1228	2828	0.27%	0.038%
41	6.698	1741	1744	1749	rBV	156	100	0.01%	0.001%
42	6.746	1754	1759	1762	rBV2	151	121	0.01%	0.002%
43	6.933	1815	1817	1820	rBV	74	38	0.00%	0.001%
44	7.010	1830	1841	1872	rBV	129871	233599	22.28%	3.101%
45	7.158	1881	1887	1899	rVB6	2493	4164	0.40%	0.055%
46	7.212	1903	1904	1908	rVB	274	126	0.01%	0.002%
47	7.235	1908	1911	1913	rBV	201	120	0.01%	0.002%
48	7.254	1915	1917	1923	rVB3	194	141	0.01%	0.002%
49	7.338	1930	1943	1983	rBV	485105	833206	79.46%	11.062%
50	7.579	2015	2018	2022	rVB2	304	187	0.02%	0.002%
51	7.643	2027	2038	2060	rBV	97232	167042	15.93%	2.218%
52	7.791	2082	2084	2085	rBV	311	114	0.01%	0.002%
53	7.852	2101	2103	2106	rBV2	182	86	0.01%	0.001%
54	7.961	2128	2137	2148	rBV3	1405	2274	0.22%	0.030%
55	8.058	2164	2167	2170	rBV	133	81	0.01%	0.001%
56	8.109	2172	2183	2217	rBV	260589	451197	43.03%	5.990%
57	8.447	2285	2288	2291	rBV2	207	144	0.01%	0.002%
58	8.460	2291	2292	2294	rVV	143	54	0.01%	0.001%
59	8.473	2294	2296	2301	rVV2	154	66	0.01%	0.001%
60	8.547	2316	2319	2325	rVB2	247	183	0.02%	0.002%
61	8.875	2409	2421	2441	rBV	372691	599492	57.17%	7.959%
62	9.077	2481	2484	2490	rBV2	161	107	0.01%	0.001%
63	9.141	2501	2504	2506	rBV	201	125	0.01%	0.002%
64	9.206	2521	2524	2527	rBV2	104	72	0.01%	0.001%
65	9.383	2576	2579	2586	rBB	129	125	0.01%	0.002%
66	9.746	2687	2692	2695	rBV	240	192	0.02%	0.003%
67	9.762	2695	2697	2705	rVV2	232	245	0.02%	0.003%
68	9.839	2718	2721	2725	rBV2	452	323	0.03%	0.004%
69	10.029	2776	2780	2783	rBV2	193	145	0.01%	0.002%
70	10.238	2833	2845	2862	rBV	313091	490879	46.82%	6.517%
71	10.402	2889	2896	2904	rBV2	1510	2294	0.22%	0.030%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091720\
Data File : VV018272.D
Acq On : 17 Sep 2020 12:43
Operator : SY/MD
Sample : L4012-15RE
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWT3RE

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Title : VOC Analysis

72	10.691	2980	2986	2989	rBV2	165	193	0.02%	0.003%
73	10.852	3033	3036	3038	rBV	107	78	0.01%	0.001%
74	11.125	3117	3121	3124	rBV3	262	215	0.02%	0.003%
75	11.174	3130	3136	3145	rBV3	4751	6729	0.64%	0.089%
76	11.270	3155	3166	3185	rBV	379918	580571	55.37%	7.708%
77	11.556	3250	3255	3267	rBV5	1165	1815	0.17%	0.024%
78	11.646	3270	3283	3306	rBV	519719	806594	76.93%	10.708%
79	11.977	3384	3386	3389	rVB2	258	128	0.01%	0.002%
80	12.042	3403	3406	3409	rBV2	193	113	0.01%	0.002%
81	12.370	3499	3508	3526	rVB2	16752	25729	2.45%	0.342%
82	13.289	3792	3794	3796	rBV	402	258	0.02%	0.003%


Sum of corrected areas: 7532377

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091720\
Data File : VV018272.D
Acq On : 17 Sep 2020 12:43
Operator : SY/MD
Sample : L4012-15RE
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWT3RE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

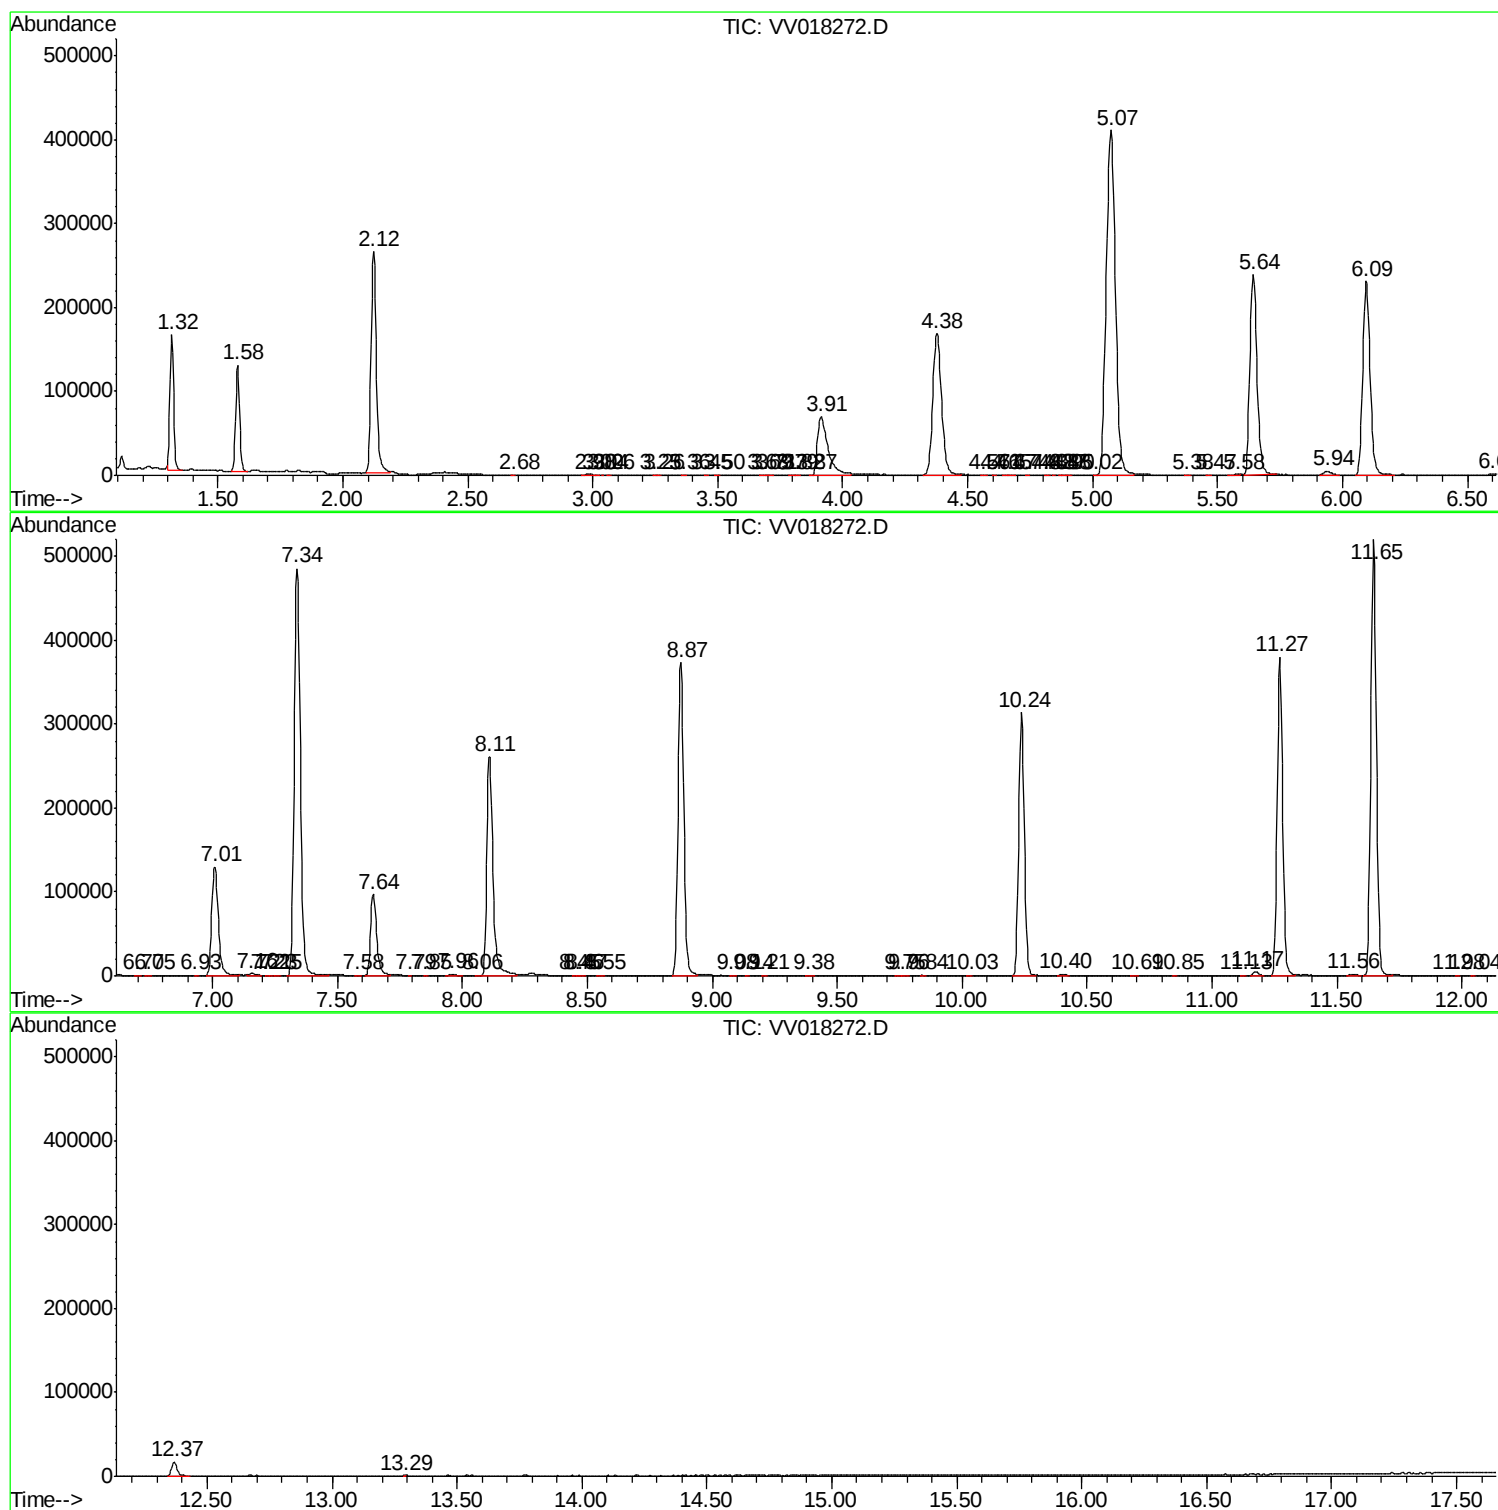

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV091720\
Data File : VV018272.D
Acq On : 17 Sep 2020 12:43
Operator : SY/MD
Sample : L4012-15RE
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWT3RE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV091720\
Data File : VV018272.D
Acq On : 17 Sep 2020 12:43
Operator : SY/MD
Sample : L4012-15RE
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BFWT3RE

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc