

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091720\
 Data File : VV018280.D
 Acq On : 17 Sep 2020 15:44
 Operator : SY/MD
 Sample : L4066-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWS4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	82	rVB	130637	130070	15.26%	2.022%
2	1.579	145	152	164	rVB	105173	115777	13.58%	1.800%
3	2.123	311	321	365	rVB	212837	336064	39.42%	5.224%
4	2.303	373	377	378	rBV	459	364	0.04%	0.006%
5	2.894	558	561	563	rBV	107	74	0.01%	0.001%
6	2.965	580	583	584	rBV	264	156	0.02%	0.002%
7	3.058	609	612	614	rBV	273	206	0.02%	0.003%
8	3.113	627	629	633	rVB2	79	44	0.01%	0.001%
9	3.171	644	647	649	rBV	99	72	0.01%	0.001%
10	3.293	682	685	686	rBV	60	35	0.00%	0.001%
11	3.309	686	690	693	rVV	179	146	0.02%	0.002%
12	3.412	718	722	726	rBV2	196	146	0.02%	0.002%
13	3.557	765	767	770	rBV	79	52	0.01%	0.001%
14	3.598	776	780	788	rVB2	115	136	0.02%	0.002%
15	3.640	788	793	797	rBV2	91	81	0.01%	0.001%
16	3.666	797	801	804	rBV	102	76	0.01%	0.001%
17	3.724	817	819	822	rVB	117	66	0.01%	0.001%
18	3.804	838	844	846	rBV2	259	246	0.03%	0.004%
19	3.917	868	879	907	rBV	52817	156452	18.35%	2.432%
20	4.377	1006	1022	1049	rBV	135986	333582	39.13%	5.186%
21	4.595	1087	1090	1095	rBV2	122	132	0.02%	0.002%
22	4.708	1122	1125	1127	rBV	77	52	0.01%	0.001%
23	4.724	1127	1130	1134	rVB2	131	79	0.01%	0.001%
24	4.762	1139	1142	1144	rBV	64	45	0.01%	0.001%
25	4.804	1151	1155	1158	rBV2	120	88	0.01%	0.001%
26	5.074	1221	1239	1271	rBV2	335022	852543	100.00%	13.253%
27	5.348	1320	1324	1326	rBV	135	126	0.01%	0.002%
28	5.360	1326	1328	1331	rVB2	192	105	0.01%	0.002%
29	5.376	1331	1333	1334	rBV	75	35	0.00%	0.001%
30	5.511	1373	1375	1378	rVB2	253	136	0.02%	0.002%
31	5.534	1378	1382	1383	rBV	150	98	0.01%	0.002%
32	5.557	1387	1389	1390	rBV	102	36	0.00%	0.001%
33	5.643	1403	1416	1441	rBV	241032	482685	56.62%	7.504%
34	5.933	1497	1506	1521	rVB2	2700	5948	0.70%	0.092%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091720\
 Data File : VV018280.D
 Acq On : 17 Sep 2020 15:44
 Operator : SY/MD
 Sample : L4066-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWS4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

35	6.032	1535	1537	1539	rBV2	162	69	0.01%	0.001%
36	6.093	1543	1556	1590	rBV	189589	384687	45.12%	5.980%
37	6.235	1597	1600	1604	rBV3	323	248	0.03%	0.004%
38	6.270	1609	1611	1614	rBV	183	89	0.01%	0.001%
39	6.296	1616	1619	1622	rVB	172	85	0.01%	0.001%
40	6.540	1693	1695	1698	rBV	76	38	0.00%	0.001%
41	6.573	1701	1705	1707	rBV2	123	77	0.01%	0.001%
42	6.595	1708	1712	1714	rBV2	286	219	0.03%	0.003%
43	6.704	1743	1746	1752	rBB2	101	95	0.01%	0.001%
44	6.801	1773	1776	1780	rVB2	107	76	0.01%	0.001%
45	6.827	1780	1784	1788	rBV2	156	127	0.01%	0.002%
46	6.846	1788	1790	1793	rBV	164	65	0.01%	0.001%
47	6.897	1803	1806	1812	rVB2	122	116	0.01%	0.002%
48	6.952	1819	1823	1827	rVB2	81	63	0.01%	0.001%
49	7.010	1829	1841	1864	rBV	103402	186896	21.92%	2.905%
50	7.187	1893	1896	1898	rVB2	88	51	0.01%	0.001%
51	7.251	1910	1916	1918	rBV2	126	127	0.01%	0.002%
52	7.338	1931	1943	1967	rBV	385751	664176	77.91%	10.325%
53	7.595	2021	2023	2025	rBV	156	104	0.01%	0.002%
54	7.643	2028	2038	2069	rVV	76122	132021	15.49%	2.052%
55	7.820	2090	2093	2094	rBV	149	67	0.01%	0.001%
56	7.846	2098	2101	2106	rVB2	222	159	0.02%	0.002%
57	7.965	2132	2138	2143	rBV2	336	475	0.06%	0.007%
58	8.016	2151	2154	2157	rBV2	133	72	0.01%	0.001%
59	8.071	2168	2171	2173	rBV	100	70	0.01%	0.001%
60	8.109	2173	2183	2219	rBV	205618	361361	42.39%	5.618%
61	8.376	2264	2266	2269	rVB2	252	118	0.01%	0.002%
62	8.399	2269	2273	2278	rVV2	242	283	0.03%	0.004%
63	8.421	2278	2280	2284	rVB	215	90	0.01%	0.001%
64	8.508	2304	2307	2309	rBV2	82	55	0.01%	0.001%
65	8.521	2309	2311	2319	rVB	238	177	0.02%	0.003%
66	8.563	2319	2324	2327	rBV2	148	145	0.02%	0.002%
67	8.589	2329	2332	2334	rBV	82	57	0.01%	0.001%
68	8.601	2334	2336	2338	rVB2	123	51	0.01%	0.001%
69	8.666	2354	2356	2358	rBV2	146	36	0.00%	0.001%
70	8.682	2359	2361	2363	rBV	76	44	0.01%	0.001%
71	8.759	2382	2385	2388	rBV	159	92	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091720\
 Data File : VV018280.D
 Acq On : 17 Sep 2020 15:44
 Operator : SY/MD
 Sample : L4066-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWS4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

72	8.875	2408	2421	2448	rBV	378238	614964	72.13%	9.560%
73	9.068	2477	2481	2485	rBV2	105	124	0.01%	0.002%
74	9.177	2507	2515	2518	rBV3	403	467	0.05%	0.007%
75	9.277	2543	2546	2549	rBV2	139	86	0.01%	0.001%
76	9.572	2636	2638	2641	rVB	163	87	0.01%	0.001%
77	9.621	2649	2653	2656	rBV	140	128	0.02%	0.002%
78	9.662	2661	2666	2669	rBV	134	124	0.01%	0.002%
79	9.765	2696	2698	2700	rBV	166	71	0.01%	0.001%
80	9.804	2707	2710	2713	rBV	121	104	0.01%	0.002%
81	9.843	2715	2722	2727	rVB4	627	854	0.10%	0.013%
82	9.933	2746	2750	2752	rBV	112	91	0.01%	0.001%
83	10.019	2774	2777	2779	rBV	96	65	0.01%	0.001%
84	10.093	2795	2800	2805	rBV	177	229	0.03%	0.004%
85	10.238	2833	2845	2868	rBV	257784	401844	47.13%	6.247%
86	10.347	2877	2879	2883	rBV2	125	73	0.01%	0.001%
87	10.396	2889	2894	2896	rBV3	329	314	0.04%	0.005%
88	10.434	2903	2906	2909	rBV2	116	95	0.01%	0.001%
89	10.582	2948	2952	2954	rBV	148	110	0.01%	0.002%
90	10.900	3048	3051	3055	rVB2	197	143	0.02%	0.002%
91	10.923	3055	3058	3060	rBV2	111	85	0.01%	0.001%
92	10.974	3071	3074	3076	rBV2	141	91	0.01%	0.001%
93	11.174	3130	3136	3144	rBV3	3214	4726	0.55%	0.073%
94	11.270	3155	3166	3196	rBV	386091	592852	69.54%	9.216%
95	11.412	3208	3210	3214	rBV	162	104	0.01%	0.002%
96	11.560	3251	3256	3257	rBV2	645	492	0.06%	0.008%
97	11.646	3270	3283	3307	rBV	414607	651739	76.45%	10.132%
98	11.868	3350	3352	3354	rBV2	130	53	0.01%	0.001%
99	12.370	3500	3508	3519	rBV4	8971	13594	1.59%	0.211%
100	13.296	3793	3796	3800	rBV3	240	191	0.02%	0.003%


Sum of corrected areas: 6432634

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091720\
Data File : VV018280.D
Acq On : 17 Sep 2020 15:44
Operator : SY/MD
Sample : L4066-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWS4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

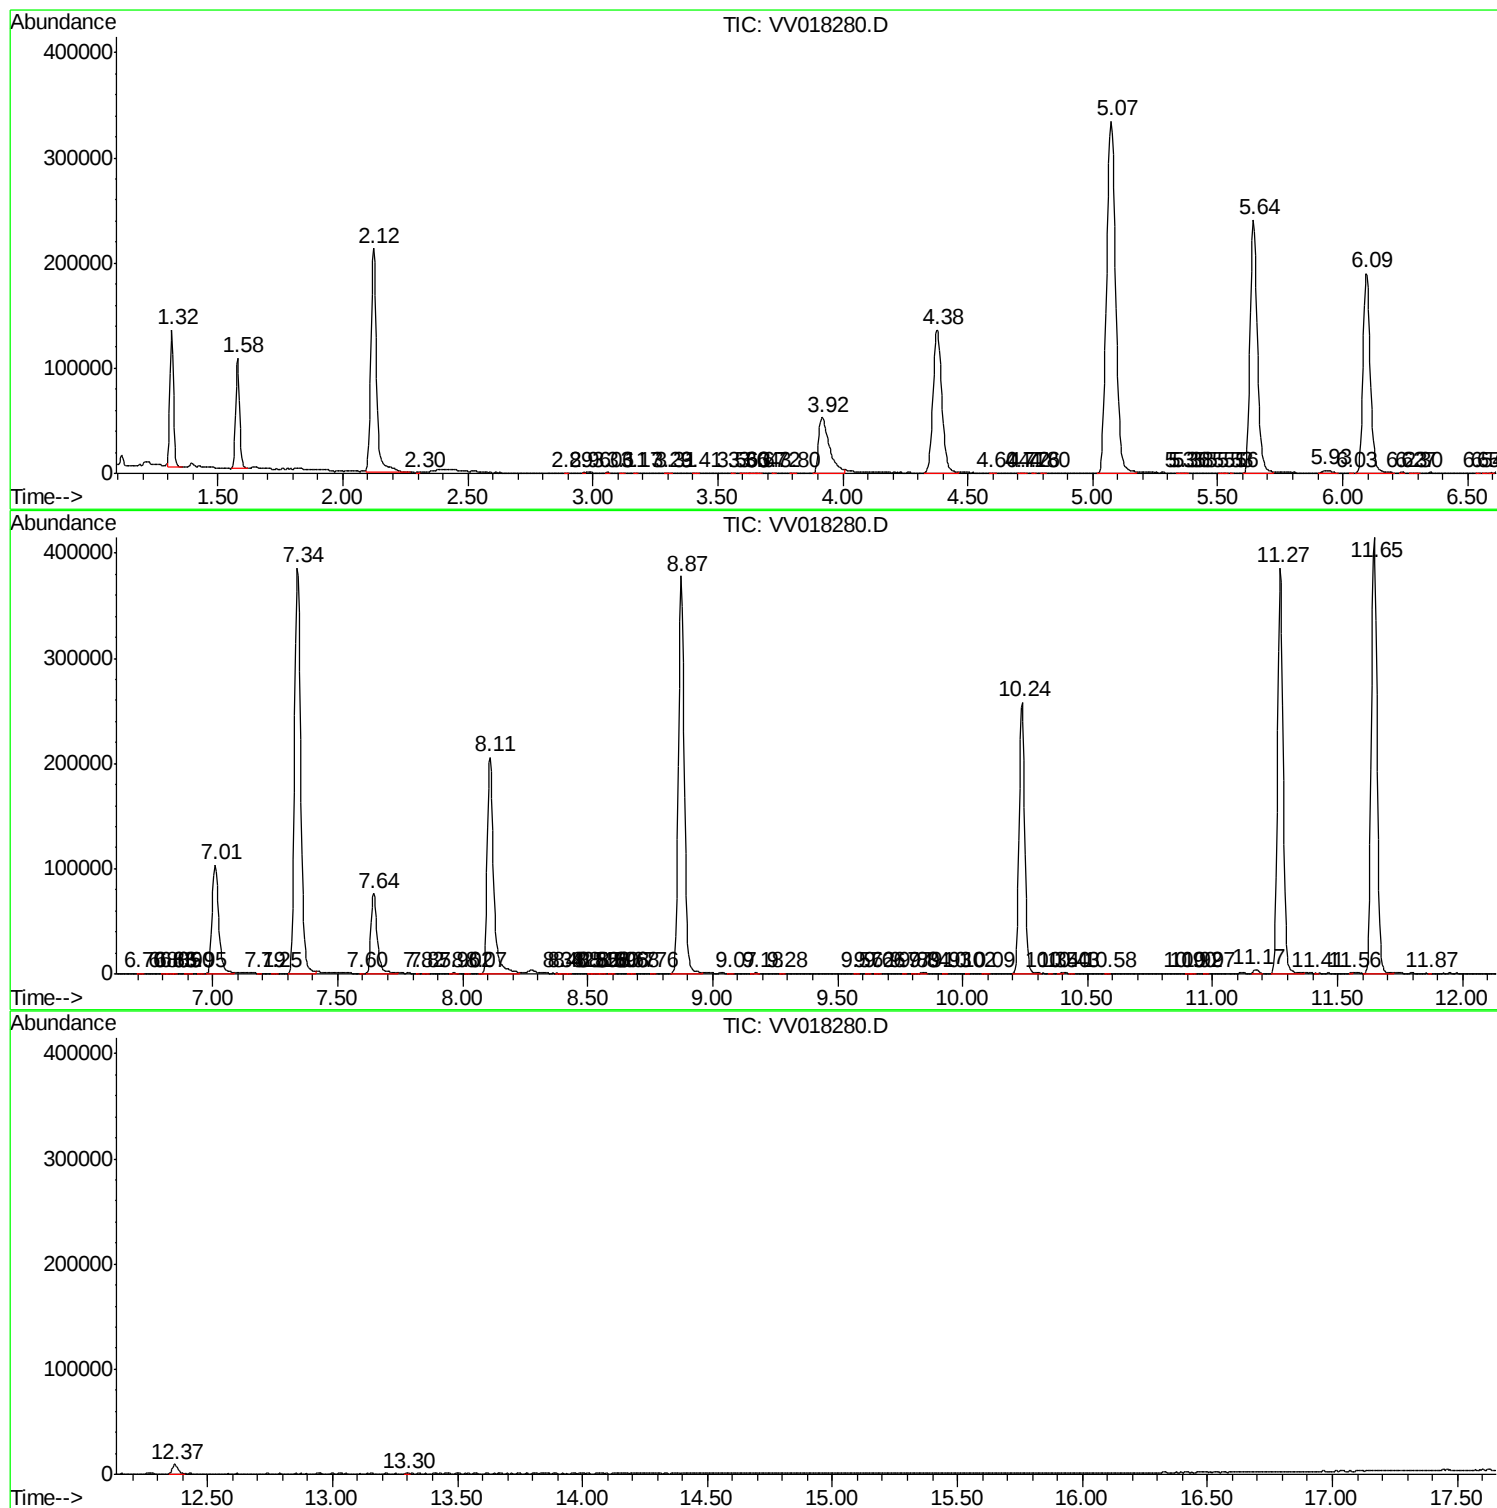

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091720\
Data File : VV018280.D
Acq On : 17 Sep 2020 15:44
Operator : SY/MD
Sample : L4066-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWS4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091720\
Data File : VV018280.D
Acq On : 17 Sep 2020 15:44
Operator : SY/MD
Sample : L4066-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWS4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc