

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091720\
 Data File : VV018290.D
 Acq On : 17 Sep 2020 19:29
 Operator : SY/MD
 Sample : L4043-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	81	rVB	127709	127394	13.57%	1.698%
2	1.576	144	151	165	rVB	110271	121959	12.99%	1.625%
3	2.119	310	320	358	rVB	224510	349067	37.17%	4.652%
4	2.412	409	411	412	rBV	360	131	0.01%	0.002%
5	2.685	493	496	497	rBV	133	73	0.01%	0.001%
6	2.785	524	527	533	rVB3	340	286	0.03%	0.004%
7	3.148	634	640	645	rVB2	194	236	0.03%	0.003%
8	3.174	645	648	652	rBV	122	84	0.01%	0.001%
9	3.209	653	659	661	rBV2	241	270	0.03%	0.004%
10	3.331	694	697	698	rBV	94	55	0.01%	0.001%
11	3.653	794	797	800	rBV2	219	199	0.02%	0.003%
12	3.679	801	805	811	rVV	170	244	0.03%	0.003%
13	3.917	868	879	929	rBV	60719	197444	21.03%	2.631%
14	4.180	959	961	966	rBV2	179	135	0.01%	0.002%
15	4.373	1004	1021	1053	rBV	151434	371391	39.55%	4.949%
16	4.531	1068	1070	1073	rVB2	212	87	0.01%	0.001%
17	4.589	1084	1088	1093	rVB3	310	222	0.02%	0.003%
18	4.624	1097	1099	1104	rVV2	214	185	0.02%	0.002%
19	4.643	1104	1105	1107	rVB	135	28	0.00%	0.000%
20	4.701	1120	1123	1124	rBV	144	64	0.01%	0.001%
21	4.749	1136	1138	1142	rBV2	145	82	0.01%	0.001%
22	4.862	1170	1173	1176	rVB2	128	82	0.01%	0.001%
23	5.000	1213	1216	1219	rBV2	121	72	0.01%	0.001%
24	5.071	1220	1238	1267	rBV2	369350	939003	100.00%	12.514%
25	5.341	1320	1322	1326	rBV2	145	69	0.01%	0.001%
26	5.376	1331	1333	1335	rBV	151	102	0.01%	0.001%
27	5.437	1350	1352	1357	rVB2	198	107	0.01%	0.001%
28	5.518	1376	1377	1379	rVB2	88	32	0.00%	0.000%
29	5.640	1403	1415	1444	rBV	331301	657424	70.01%	8.761%
30	5.933	1495	1506	1521	rVV3	3545	6876	0.73%	0.092%
31	5.984	1521	1522	1526	rVB	144	57	0.01%	0.001%
32	6.093	1543	1556	1582	rBV	209726	424440	45.20%	5.656%
33	6.215	1592	1594	1595	rBV	166	55	0.01%	0.001%
34	6.225	1595	1597	1599	rVV2	317	180	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091720\
 Data File : VV018290.D
 Acq On : 17 Sep 2020 19:29
 Operator : SY/MD
 Sample : L4043-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

35	6.251	1602	1605	1610	rVB2	478	385	0.04%	0.005%
36	6.531	1689	1692	1694	rBV2	117	78	0.01%	0.001%
37	6.733	1752	1755	1759	rVB2	123	82	0.01%	0.001%
38	6.830	1782	1785	1788	rBV	78	51	0.01%	0.001%
39	7.010	1830	1841	1870	rBV	113079	206198	21.96%	2.748%
40	7.190	1895	1897	1899	rVB	148	78	0.01%	0.001%
41	7.241	1910	1913	1917	rVB3	184	135	0.01%	0.002%
42	7.293	1928	1929	1930	rBV3	126	36	0.00%	0.000%
43	7.338	1930	1943	1966	rBV	429957	735392	78.32%	9.800%
44	7.643	2028	2038	2060	rBV	85045	145307	15.47%	1.936%
45	7.833	2095	2097	2099	rVB	173	70	0.01%	0.001%
46	7.855	2099	2104	2110	rBV2	233	237	0.03%	0.003%
47	7.945	2129	2132	2133	rBV	274	152	0.02%	0.002%
48	8.010	2149	2152	2155	rBV2	126	94	0.01%	0.001%
49	8.109	2173	2183	2228	rBV	238931	416493	44.35%	5.550%
50	8.482	2297	2299	2301	rVB	134	33	0.00%	0.000%
51	8.598	2334	2335	2341	rVB	149	59	0.01%	0.001%
52	8.875	2408	2421	2447	rBV	515495	826949	88.07%	11.020%
53	9.103	2489	2492	2493	rBV2	97	60	0.01%	0.001%
54	9.209	2521	2525	2529	rBV2	160	176	0.02%	0.002%
55	9.412	2585	2588	2590	rBV2	119	67	0.01%	0.001%
56	9.566	2634	2636	2637	rBV2	173	62	0.01%	0.001%
57	9.675	2668	2670	2672	rBV	90	58	0.01%	0.001%
58	9.958	2755	2758	2763	rBV	154	135	0.01%	0.002%
59	10.090	2796	2799	2801	rBV	107	67	0.01%	0.001%
60	10.238	2833	2845	2865	rBV	292254	450394	47.97%	6.002%
61	10.402	2889	2896	2903	rBV2	762	946	0.10%	0.013%
62	10.569	2946	2948	2951	rVB	163	92	0.01%	0.001%
63	10.739	2998	3001	3002	rBV2	96	58	0.01%	0.001%
64	11.190	3139	3141	3143	rVB2	133	54	0.01%	0.001%
65	11.270	3155	3166	3193	rBV	529161	790094	84.14%	10.529%
66	11.646	3271	3283	3306	rBV	472848	729822	77.72%	9.726%
67	11.778	3320	3324	3325	rBV	454	214	0.02%	0.003%
68	11.839	3341	3343	3347	rBV3	221	184	0.02%	0.002%
69	12.119	3427	3430	3432	rBV2	112	73	0.01%	0.001%
70	12.325	3493	3494	3497	rBV	126	80	0.01%	0.001%
71	12.534	3556	3559	3563	rBV2	174	102	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091720\
Data File : VV018290.D
Acq On : 17 Sep 2020 19:29
Operator : SY/MD
Sample : L4043-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE0

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Title : VOC Analysis

72	13.582	3883	3885	3886	rBV2	135	36	0.00%	0.000%
73	14.025	4021	4023	4026	rVB	169	49	0.01%	0.001%
74	14.157	4061	4064	4068	rVB3	330	267	0.03%	0.004%
75	14.186	4070	4073	4075	rBV2	214	112	0.01%	0.001%
76	14.437	4147	4151	4155	rBV2	324	291	0.03%	0.004%
77	14.492	4165	4168	4171	rBV3	257	180	0.02%	0.002%
78	14.649	4214	4217	4220	rBV2	252	205	0.02%	0.003%


Sum of corrected areas: 7503842

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091720\
Data File : VV018290.D
Acq On : 17 Sep 2020 19:29
Operator : SY/MD
Sample : L4043-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0AE0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

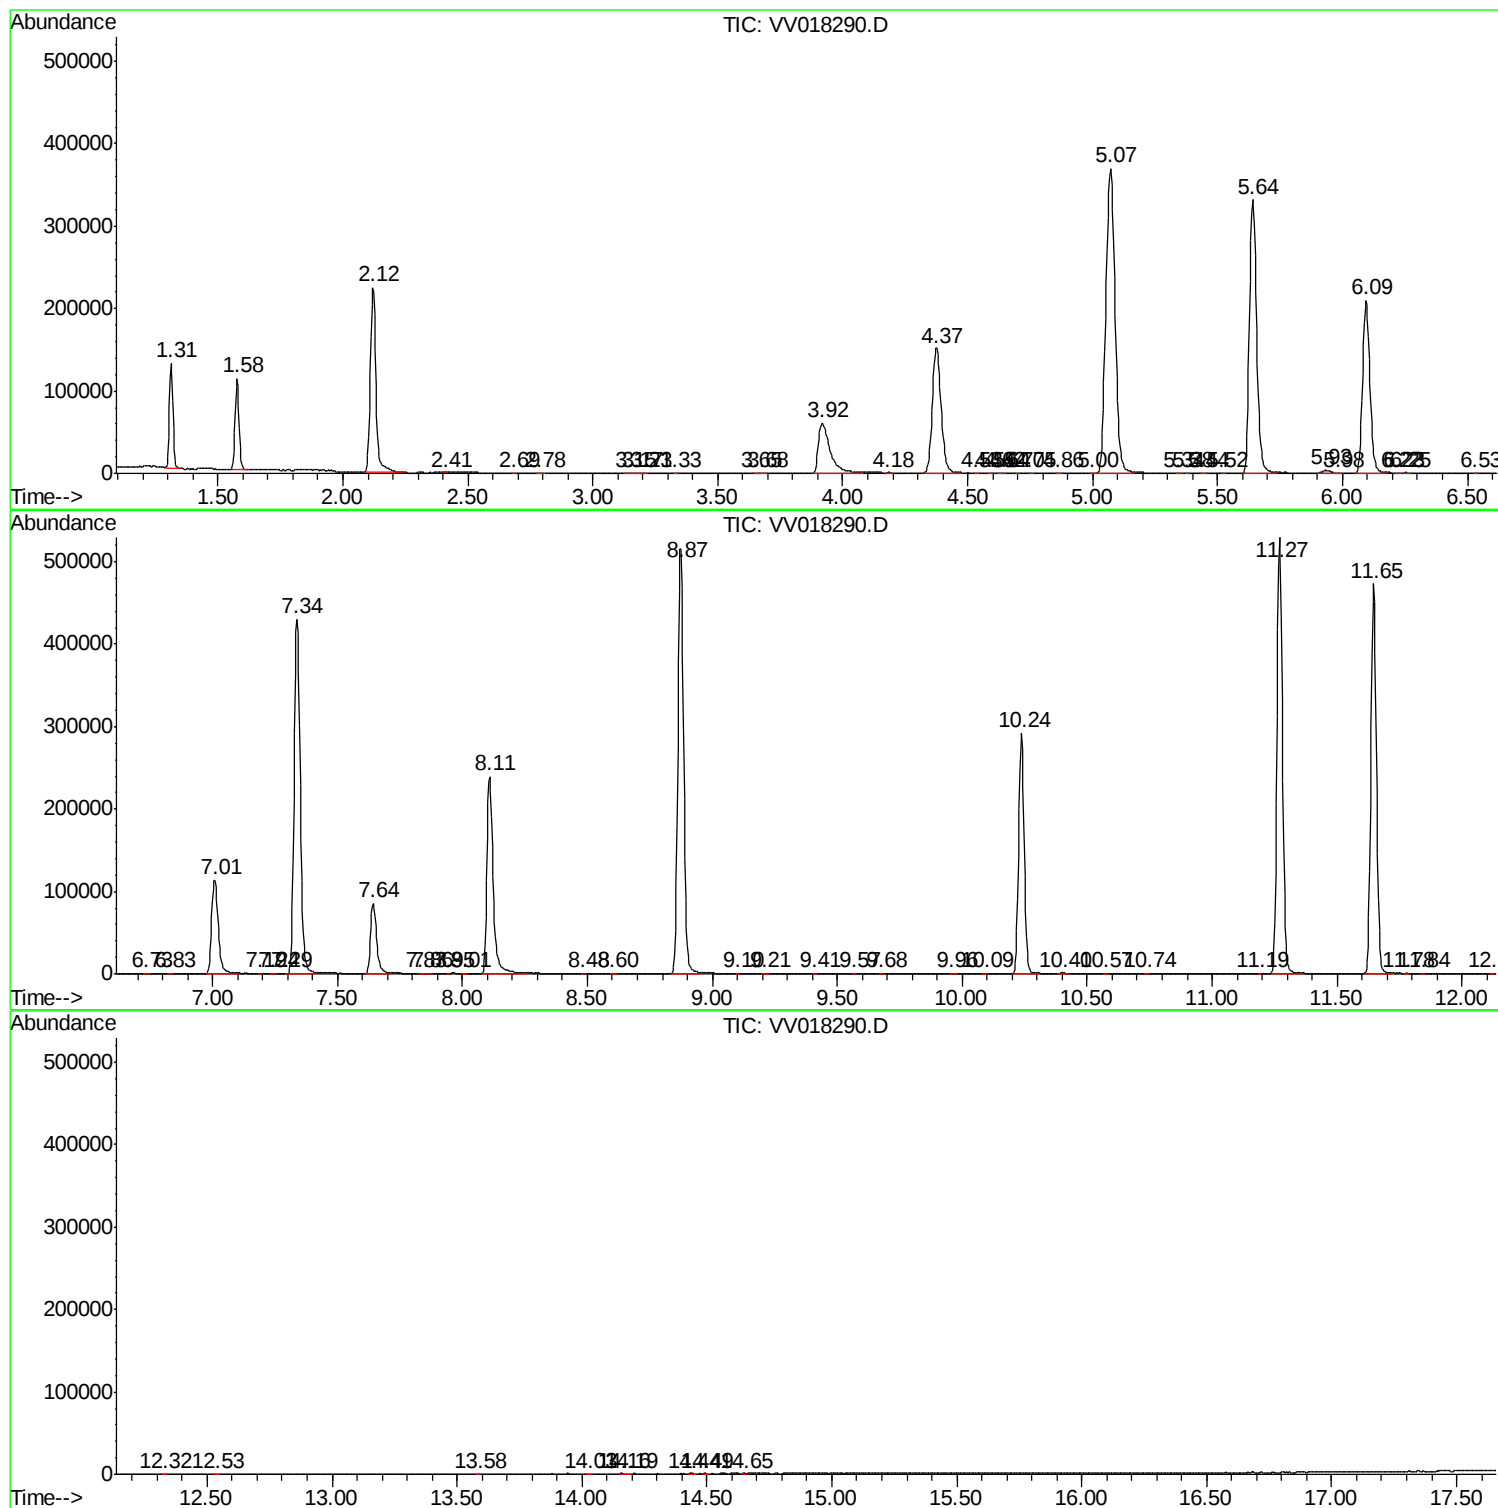

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV091720\
Data File : VV018290.D
Acq On : 17 Sep 2020 19:29
Operator : SY/MD
Sample : L4043-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091720\
Data File : VV018290.D
Acq On : 17 Sep 2020 19:29
Operator : SY/MD
Sample : L4043-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc