


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV091720\
 Data File : VV018268.D
 Acq On : 17 Sep 2020 09:44
 Operator : SY/MD
 Sample : BFB93
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB93

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis
 Last Update : Fri Sep 18 08:05:39 2020

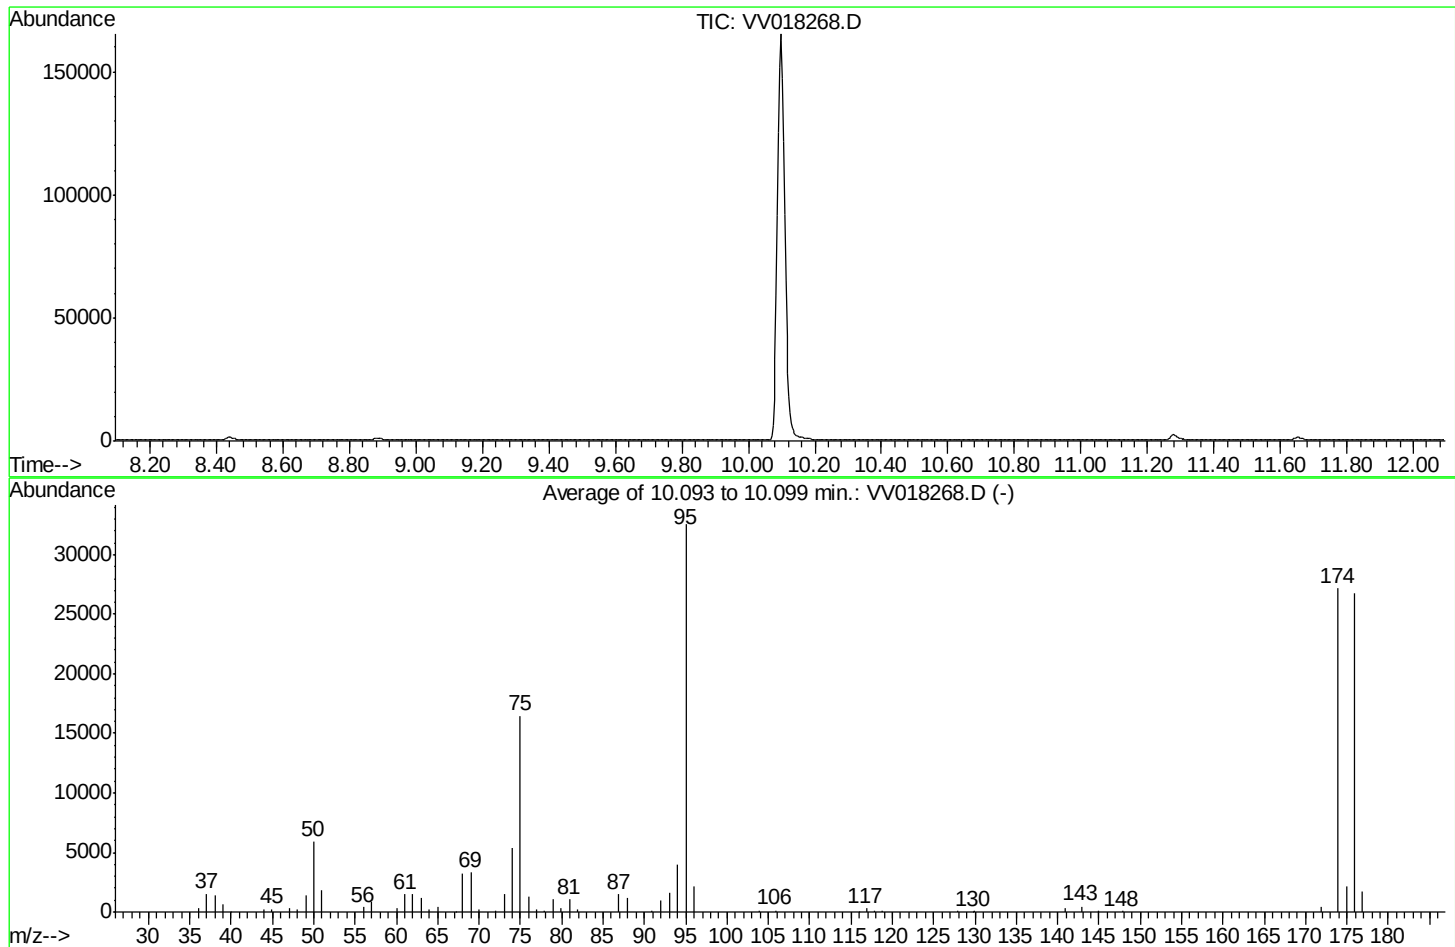

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	5887	PASS
75	95	30	80	50.6	16485	PASS
95	95	100	100	100.0	32554	PASS
96	95	5	9	6.5	2115	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.5	27181	PASS
175	174	5	9	7.8	2109	PASS
176	174	95	101	98.3	26717	PASS
177	176	5	9	6.5	1736	PASS

m/z	Abundance
36.00	294.0
37.00	1498.0
38.00	1395.0
39.00	575.0
39.90	217.0
44.00	490.0
44.90	274.0
47.00	342.0
47.90	204.0
49.00	1355.0
50.00	5683.0
51.00	1793.0
56.00	362.0
57.00	828.0
60.00	297.0
61.00	1400.0
62.00	1399.0
63.00	1226.0
63.90	214.0
65.00	361.0
68.00	3223.0
69.00	3214.0
70.00	254.0
72.00	149.0
73.00	1573.0
74.00	5230.0
75.00	15839.0
76.00	1305.0
77.00	227.0
78.00	150.0
78.90	1060.0
79.80	356.0
80.90	1074.0
81.90	261.0
86.90	1372.0
87.90	1226.0
90.90	115.0
92.00	903.0
93.00	1426.0
94.00	3751.0
95.00	31184.0
96.00	2076.0
104.00	135.0
105.90	155.0
115.90	106.0
116.90	286.0
117.80	162.0
118.80	129.0
129.70	132.0
140.80	322.0
142.90	417.0
144.90	126.0
171.90	405.0
173.90	25232.0
174.90	1960.0
175.90	24760.0
176.90	1613.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93

m/z	Abundance
36.00	330.0
37.00	1583.0
38.00	1450.0
39.00	644.0
39.90	212.0
44.00	505.0
44.90	264.0
47.00	368.0
48.00	225.0
49.00	1446.0
50.00	6084.0
51.00	1905.0
56.00	423.0
57.00	904.0
60.00	331.0
61.00	1557.0
62.00	1528.0
63.00	1264.0
63.90	233.0
65.00	406.0
67.20	112.0
68.00	3311.0
69.00	3393.0
70.00	259.0
72.00	169.0
73.00	1595.0
74.00	5601.0
75.00	16984.0
76.00	1337.0
77.00	229.0
78.00	145.0
78.90	1093.0
79.90	348.0
80.90	1096.0
81.90	257.0
86.90	1517.0
87.90	1255.0
90.90	126.0
92.00	961.0
93.00	1645.0
94.00	4115.0
95.00	33680.0
96.00	2162.0
104.00	126.0
105.90	161.0
116.90	330.0
117.80	162.0
118.80	150.0
127.90	101.0
129.90	161.0
140.80	340.0
142.90	457.0
144.90	148.0
147.90	104.0
171.90	449.0
173.90	28016.0
174.90	2169.0
175.90	27688.0
176.90	1798.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93

m/z	Abundance
36.00	344.0
37.00	1527.0
38.00	1403.0
39.00	651.0
39.90	190.0
44.00	471.0
45.00	250.0
47.00	357.0
48.00	242.0
49.00	1402.0
50.00	5894.0
51.00	1802.0
56.00	440.0
57.00	899.0
60.00	355.0
61.00	1556.0
62.00	1512.0
63.00	1187.0
63.90	235.0
65.10	378.0
68.00	3020.0
69.00	3253.0
70.00	248.0
72.00	160.0
73.00	1455.0
74.00	5414.0
75.00	16632.0
76.00	1260.0
76.90	237.0
77.80	157.0
78.90	985.0
79.90	334.0
80.90	1040.0
81.90	247.0
86.90	1510.0
87.90	1219.0
90.80	132.0
92.00	926.0
93.00	1693.0
94.00	4046.0
95.00	32800.0
96.00	2107.0
103.80	135.0
105.90	155.0
116.80	326.0
117.80	158.0
118.80	163.0
127.80	116.0
129.90	148.0
140.90	339.0
142.80	490.0
144.90	180.0
147.80	102.0
171.90	465.0
173.90	28296.0
174.90	2200.0
175.90	27704.0
176.90	1797.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93

Scan 2790 (10.061 min): VV018268.D
BFB93

m/z	Abundance
39.90	174.0
43.90	277.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93