

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022213.D
 Acq On : 18 Sep 2021 02:43
 Operator : SY/MD
 Sample : M3787-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 18 04:46:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 18 04:25:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	302053	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	290347	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	124399	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	109791	52.487	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	104.980%
7) Chloroethane-d5	1.565	69	86700	53.076	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	106.160%
11) 1,1-Dichloroethene-d2	2.105	63	150636	43.544	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.080%
21) 2-Butanone-d5	3.905	46	155562	108.439	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	108.440%
24) Chloroform-d	4.349	84	193065	50.619	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.240%
26) 1,2-Dichloroethane-d4	5.034	65	118122	52.579	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.160%
32) Benzene-d6	5.050	84	400943	50.912	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.820%
36) 1,2-Dichloropropane-d6	6.072	67	126617	51.124	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.240%
41) Toluene-d8	7.317	98	354394	47.672	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.340%
43) trans-1,3-Dichloroprop...	7.625	79	48208	40.896	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.800%
47) 2-Hexanone-d5	8.092	63	94829	99.790	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.790%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	149068	46.997	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.000%
66) 1,2-Dichlorobenzene-d4	11.629	152	125549	51.338	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.680%
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	11.252	75	13950	6.470	ug/L	# 64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022213.D
Acq On : 18 Sep 2021 02:43
Operator : SY/MD
Sample : M3787-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Sep 18 04:46:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 18 04:25:40 2021
Response via : Initial Calibration

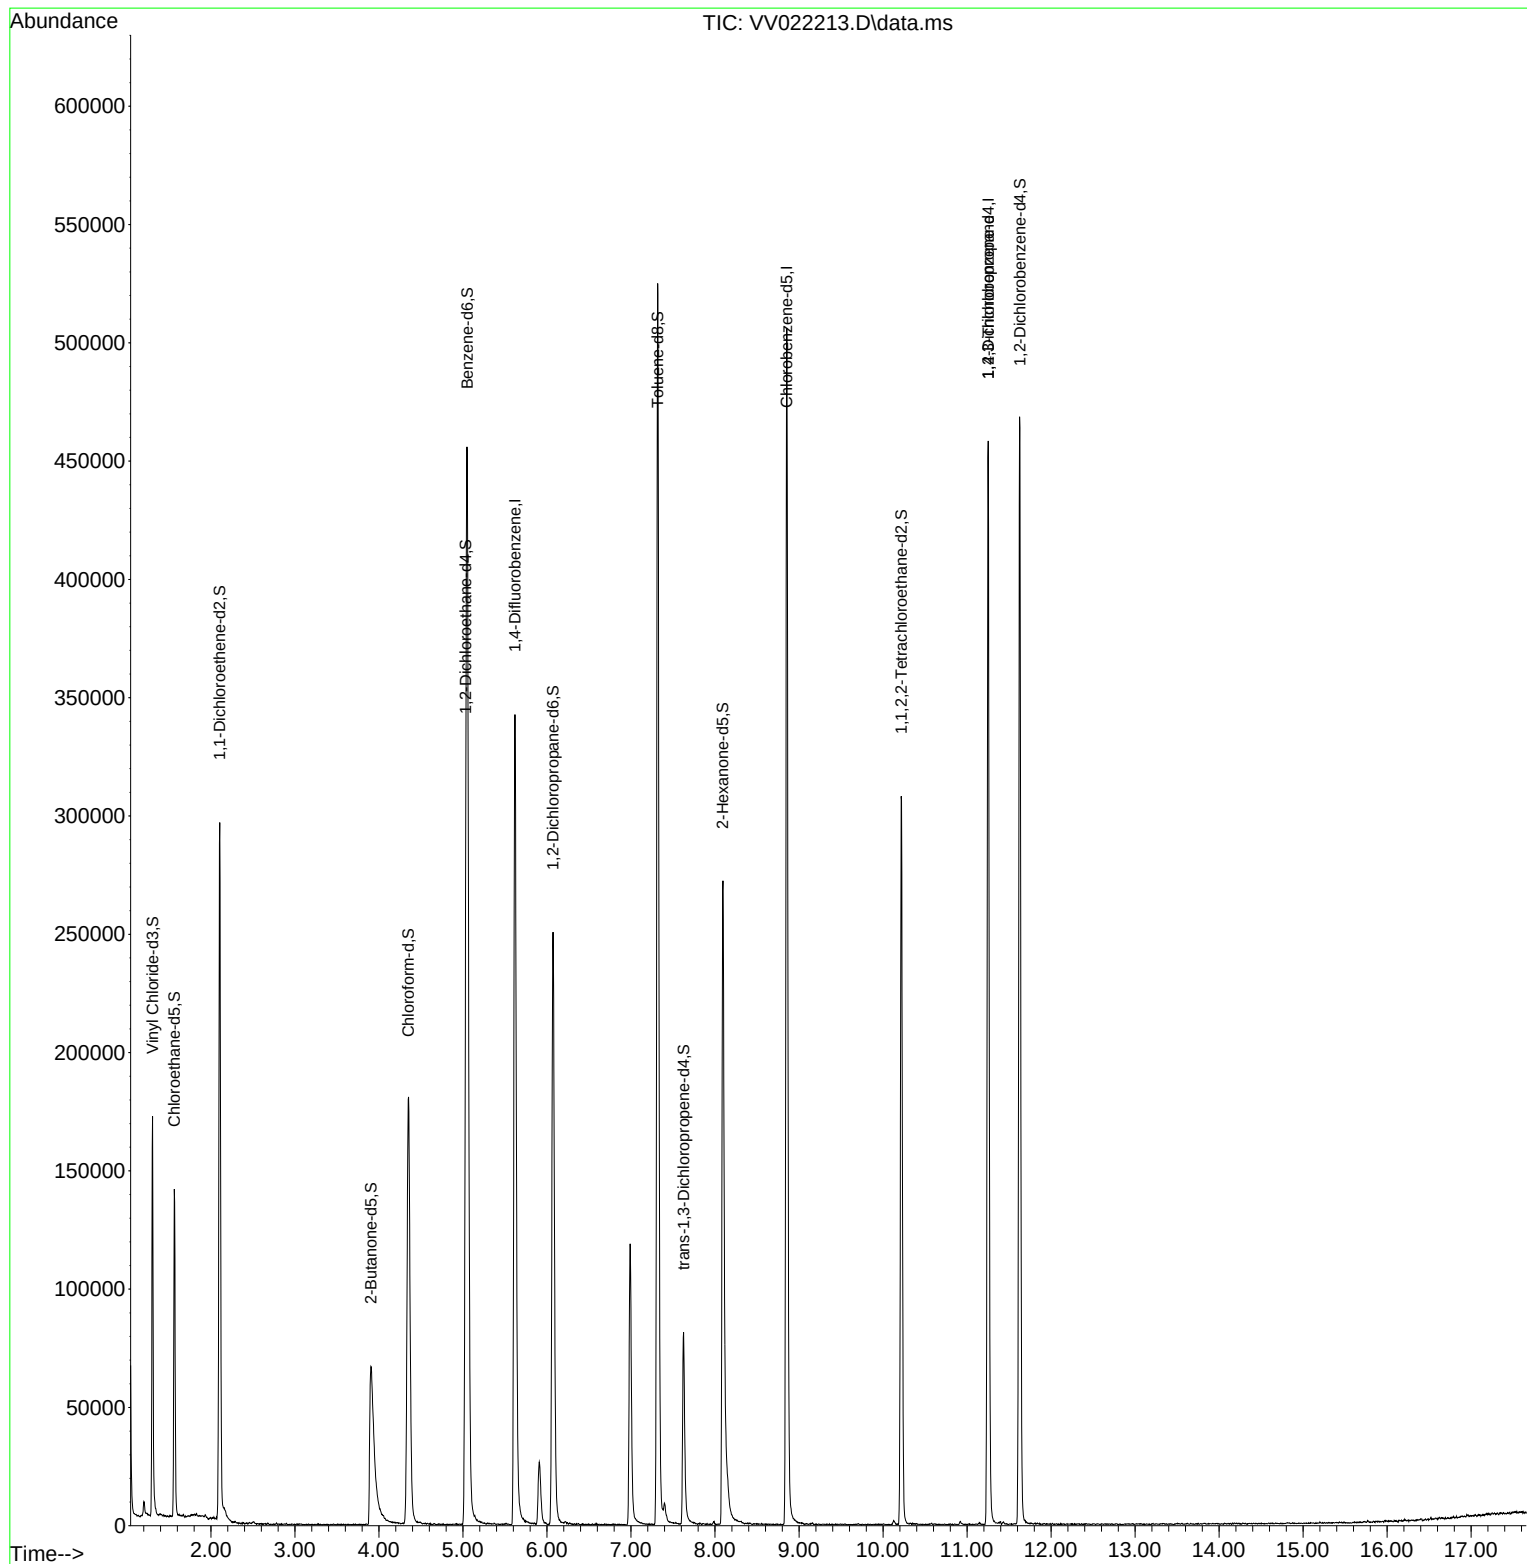

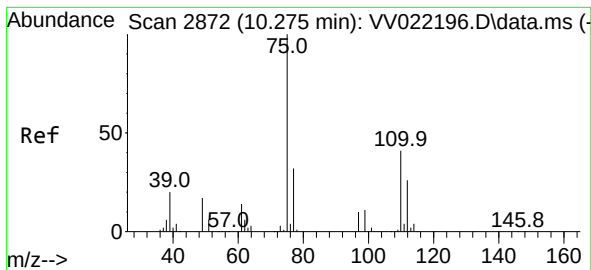

#61
 1,2,3-Trichloropropane
 Concen: 6.470 ug/L
 RT: 11.252 min Scan# 3176
 Delta R.T. 0.978 min
 Lab File: VV022213.D
 Acq: 18 Sep 2021 02:43

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 13950
 Ion Ratio Lower Upper
 75 100
 77 31.7 26.2 39.2
 110 3.0 33.8 50.6#

