

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022203.D
 Acq On : 17 Sep 2021 22:42
 Operator : SY/MD
 Sample : M3787-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CF8

Manual Integrations
 APPROVED

MMDadoda
 9/20/2021 12:19:24 PM

Quant Time: Sep 18 04:44:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 18 04:25:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	305995	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	293397	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	126550	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	113259	53.448	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	106.900%
7) Chloroethane-d5	1.564	69	89608	54.150	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	108.300%
11) 1,1-Dichloroethene-d2	2.105	63	154579	44.108	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.220%
21) 2-Butanone-d5	3.902	46	161863	111.377	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	111.380%
24) Chloroform-d	4.349	84	194859	50.431	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.860%
26) 1,2-Dichloroethane-d4	5.034	65	122190	53.689	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.380%
32) Benzene-d6	5.050	84	408780	51.368	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.740%
36) 1,2-Dichloropropane-d6	6.072	67	128258	51.249	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.500%
41) Toluene-d8	7.317	98	361452	48.116	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.240%
43) trans-1,3-Dichloroprop...	7.625	79	50789	42.638	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.280%
47) 2-Hexanone-d5	8.092	63	92990	96.838	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	96.840%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	147339	45.969	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.940%
66) 1,2-Dichlorobenzene-d4	11.625	152	131105	52.699	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.400%
Target Compounds					Qvalue	
13) Acetone	2.188	43	7347m	6.034	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022203.D
Acq On : 17 Sep 2021 22:42
Operator : SY/MD
Sample : M3787-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
C0CF8

Manual Integrations
APPROVED

MMDadoda
9/20/2021 12:19:24 PM




Quant Time: Sep 18 04:44:21 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 18 04:25:40 2021
Response via : Initial Calibration

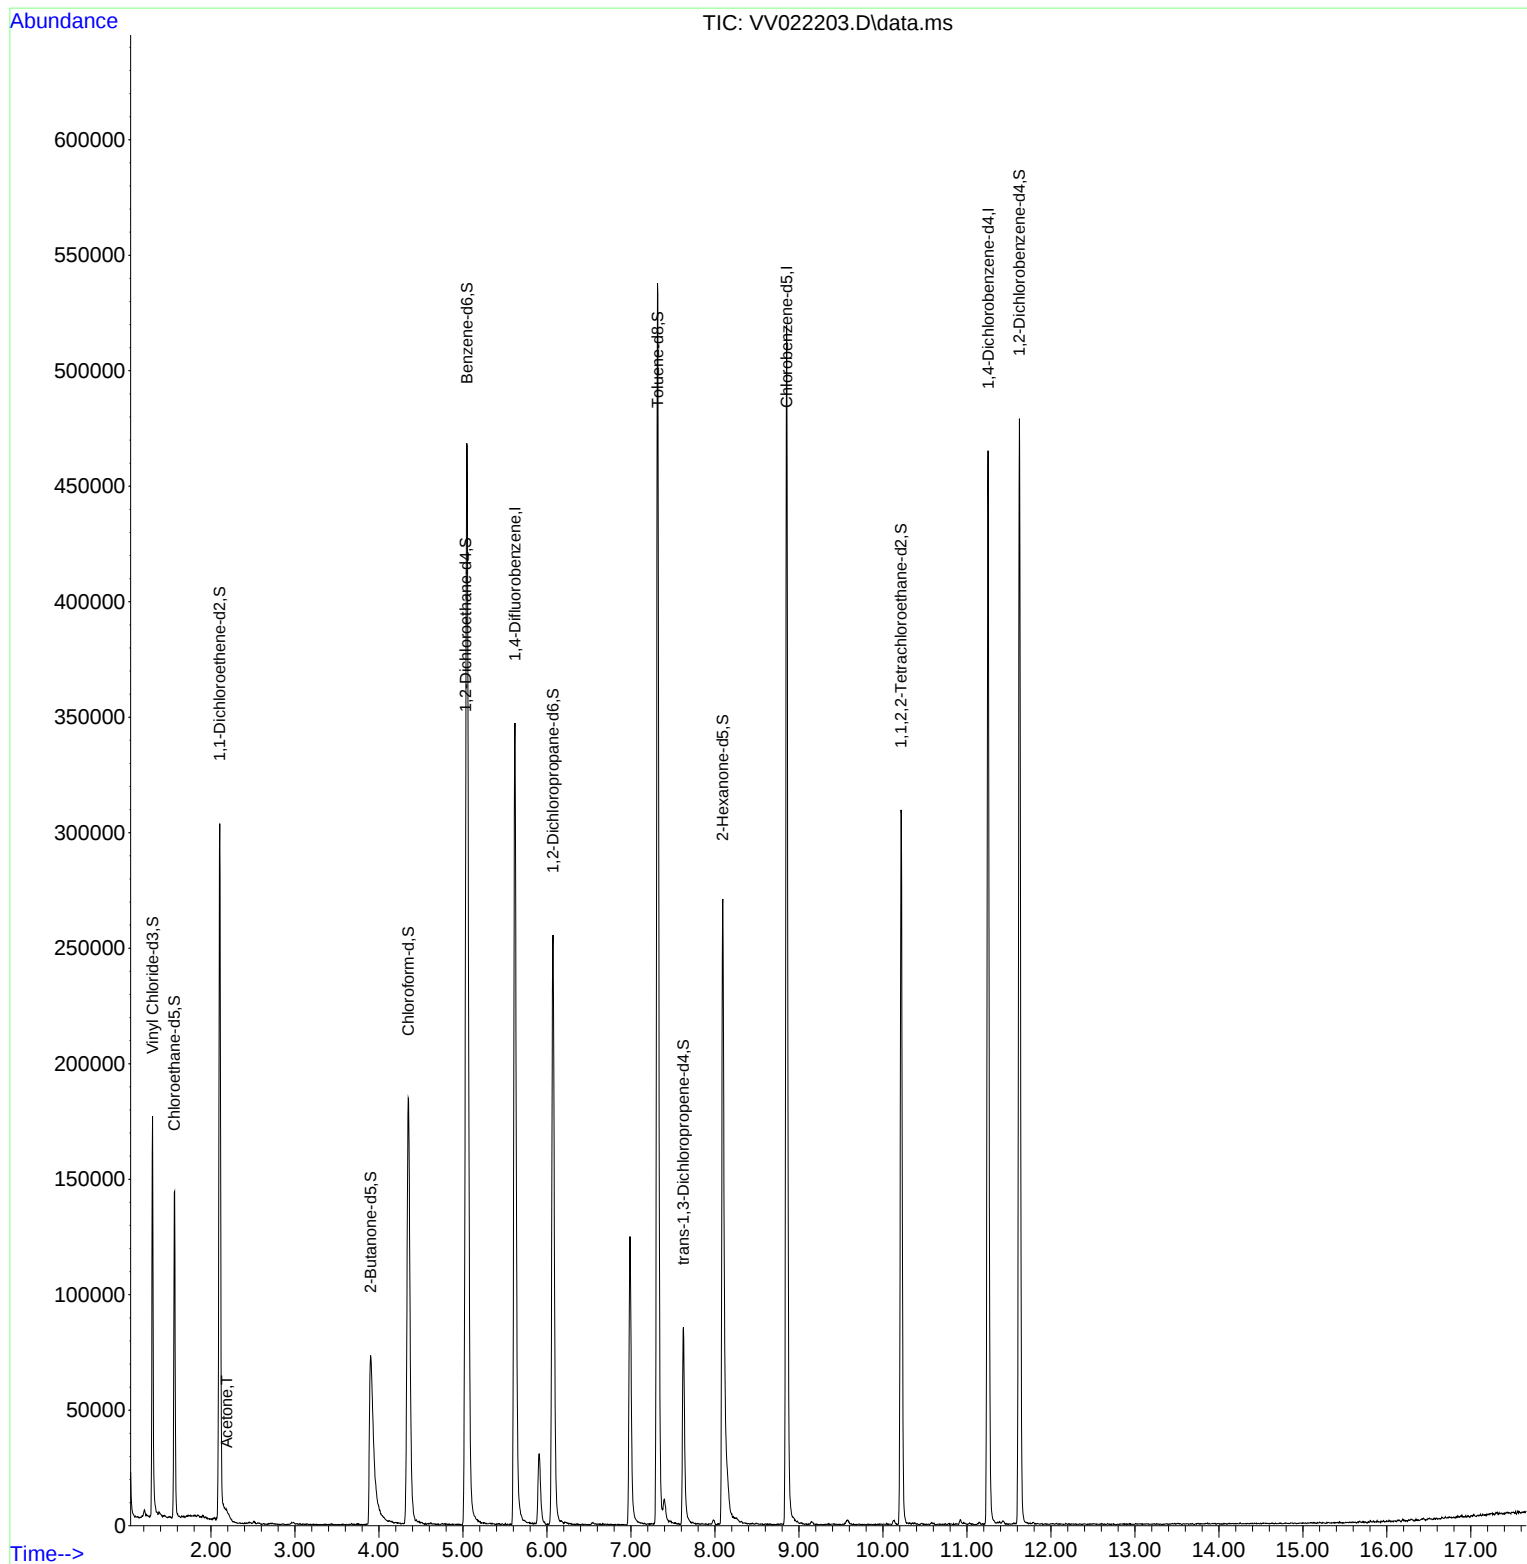

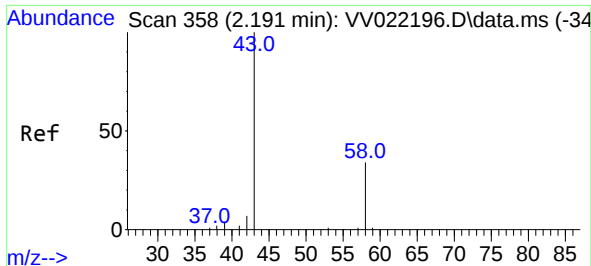

#13
Acetone
Concen: 6.034 ug/L m
RT: 2.188 min Scan# 357
Delta R.T. -0.003 min
Lab File: VV022203.D
Acq: 17 Sep 2021 22:42

Tgt Ion: 43 Resp: 7347
Ion Ratio Lower Upper
43 100
58 29.7 0.0 0.4#

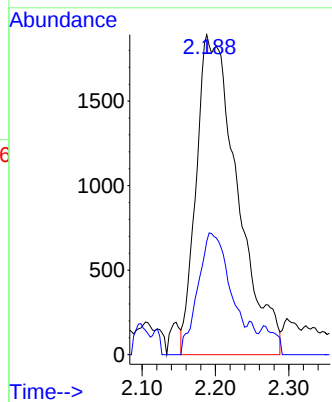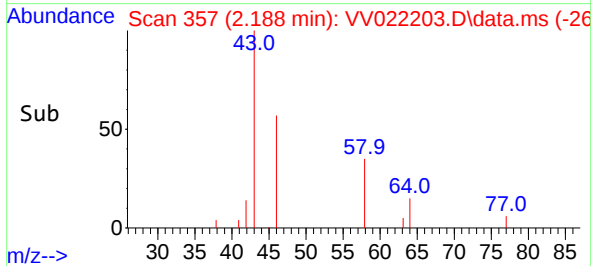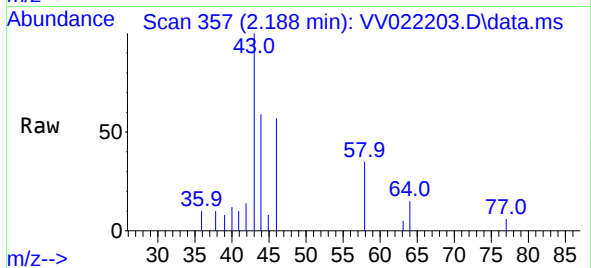

Instrument :
MSVOA_V
ClientSampleId :
C0CF8

Manual Integrations
APPROVED

MMDadoda
9/20/2021 12:19:24 PM