

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022209.D
 Acq On : 18 Sep 2021 01:06
 Operator : SY/MD
 Sample : M3787-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CG6

Quant Time: Sep 18 04:45:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 18 04:25:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	306776	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	294461	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	126418	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	110565	52.044	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 104.080%			
7) Chloroethane-d5	1.565	69	87220	52.572	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 105.140%			
11) 1,1-Dichloroethene-d2	2.105	63	153079	43.569	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 87.140%			
21) 2-Butanone-d5	3.909	46	160168	109.931	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 109.930%			
24) Chloroform-d	4.352	84	190161	49.090	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 98.180%			
26) 1,2-Dichloroethane-d4	5.034	65	117572	51.528	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 103.060%			
32) Benzene-d6	5.050	84	398691	49.919	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 99.840%			
36) 1,2-Dichloropropane-d6	6.072	67	125314	49.891	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 99.780%			
41) Toluene-d8	7.317	98	350129	46.440	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 92.880%			
43) trans-1,3-Dichloroprop...	7.625	79	48648	40.693	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 81.380%			
47) 2-Hexanone-d5	8.095	63	92695	96.182	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 96.180%			
56) 1,1,2,2-Tetrachloroeth...	10.217	84	148295	46.100	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 92.200%			
66) 1,2-Dichlorobenzene-d4	11.625	152	126499	50.900	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 101.800%			
Target Compounds					Qvalue	
12) 1,1-Dichloroethene	2.114	96	3159	1.785	ug/L #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022209.D
Acq On : 18 Sep 2021 01:06
Operator : SY/MD
Sample : M3787-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CG6

Quant Time: Sep 18 04:45:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 18 04:25:40 2021
Response via : Initial Calibration

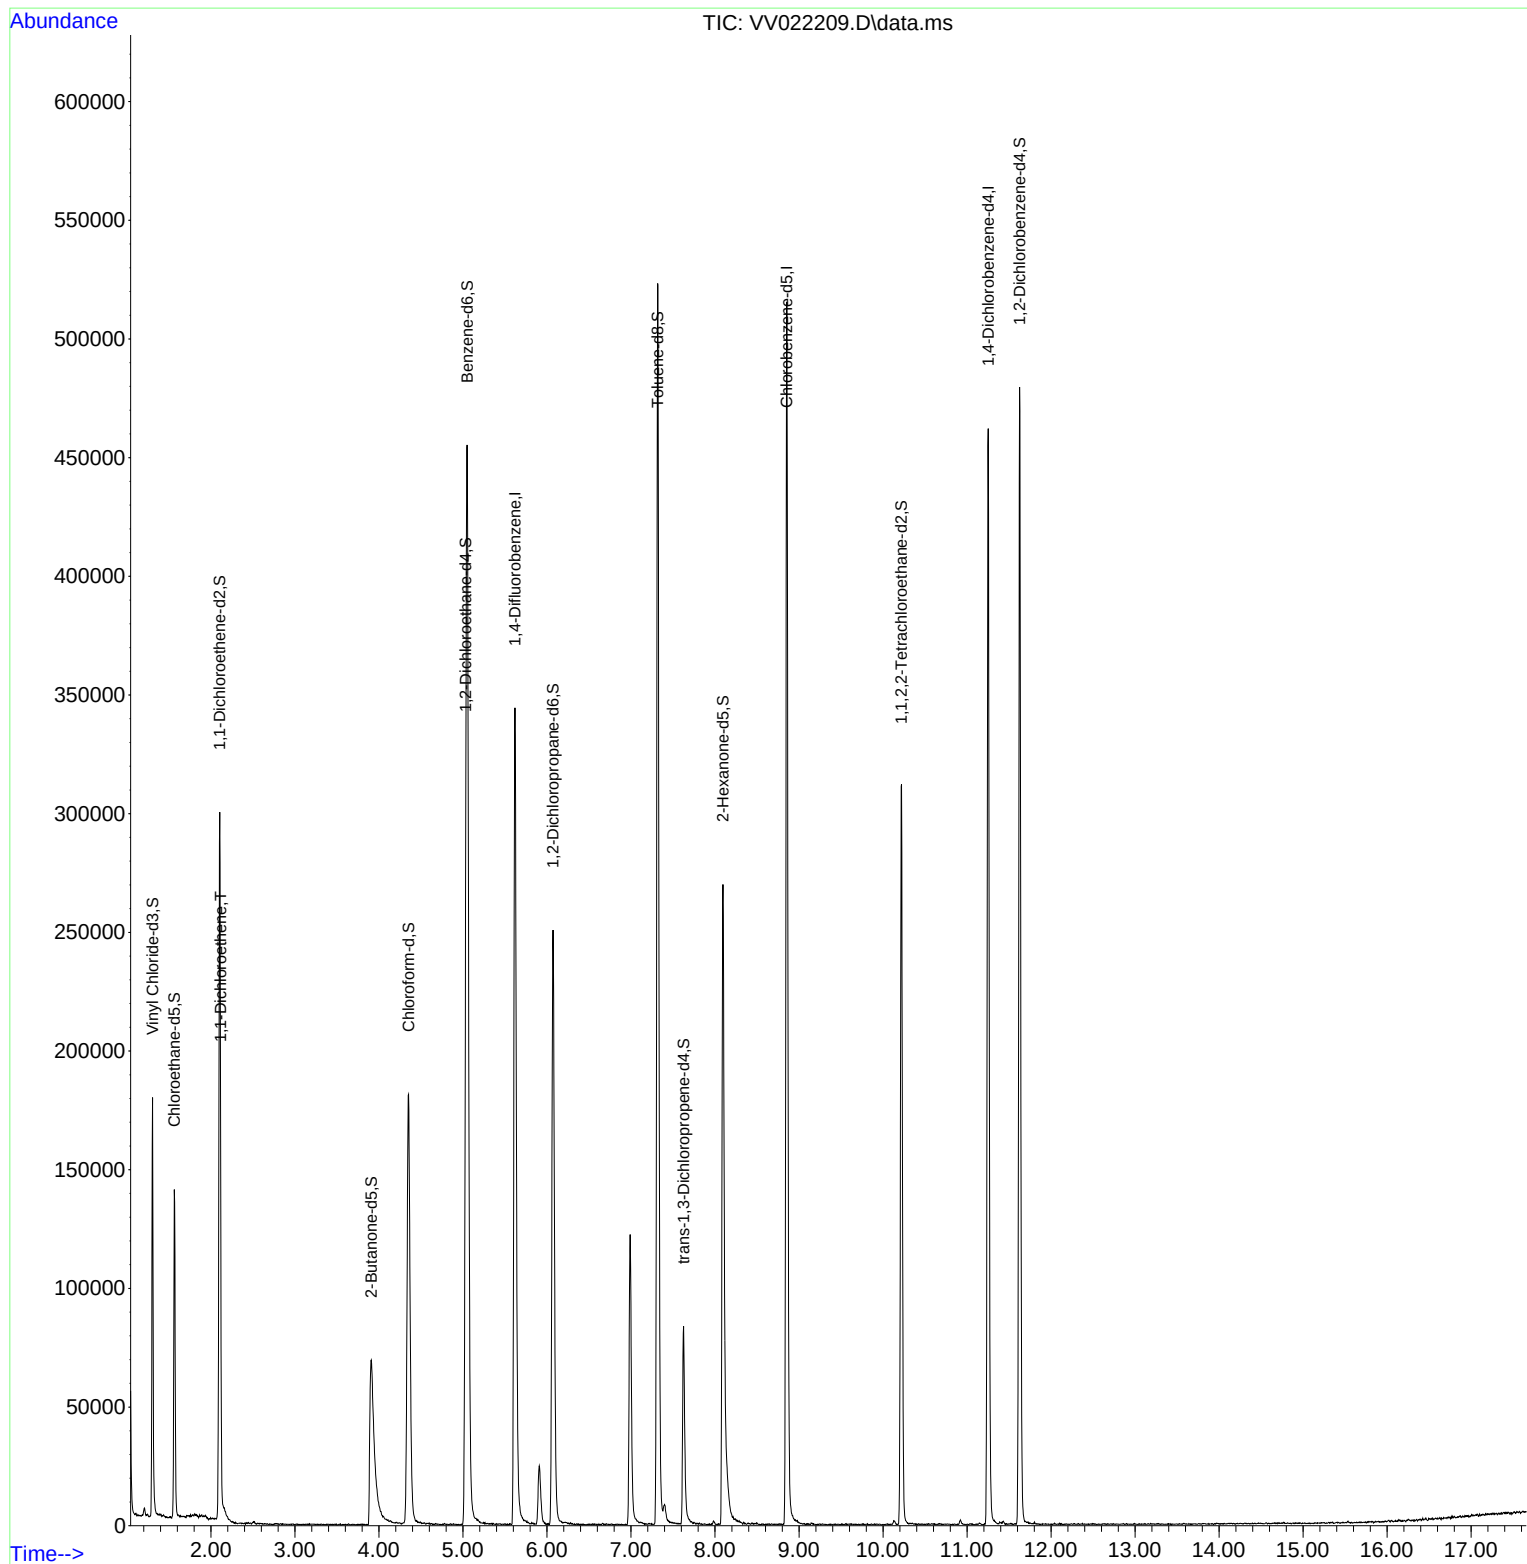

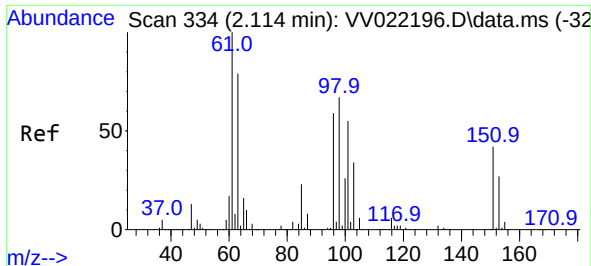

#12
 1,1-Dichloroethene
 Concen: 1.785 ug/L
 RT: 2.114 min Scan# 334
 Delta R.T. 0.000 min
 Lab File: VV022209.D
 Acq: 18 Sep 2021 01:06

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CG6

Tgt Ion: 96 Resp: 3159
 Ion Ratio Lower Upper
 96 100
 61 439.7 113.2 210.2#
 63 2936.4 102.3 189.9#

