

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022173.D
 Acq On : 17 Sep 2021 09:56
 Operator : SY/MD
 Sample : M3764-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022173.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	103	rVB	133071	139663	12.24%	1.599%
2	1.568	156	164	179	rBV	125680	140668	12.33%	1.611%
3	2.105	321	331	368	rVB	262640	401379	35.18%	4.597%
4	2.613	487	489	492	rBV2	377	320	0.03%	0.004%
5	2.686	511	512	515	rVB2	343	156	0.01%	0.002%
6	2.728	522	525	531	rBV3	257	196	0.02%	0.002%
7	2.767	531	537	539	rBV3	281	290	0.03%	0.003%
8	2.834	556	558	561	rBV2	374	224	0.02%	0.003%
9	2.863	565	567	572	rBV2	235	142	0.01%	0.002%
10	2.992	605	607	610	rVB2	469	199	0.02%	0.002%
11	3.008	610	612	614	rBV	324	162	0.01%	0.002%
12	3.069	628	631	634	rBV	239	164	0.01%	0.002%
13	3.236	680	683	684	rBV	366	150	0.01%	0.002%
14	3.259	688	690	693	rVV	308	203	0.02%	0.002%
15	3.288	697	699	704	rVB2	280	186	0.02%	0.002%
16	3.423	732	741	743	rBV2	293	426	0.04%	0.005%
17	3.661	811	815	816	rVB2	255	146	0.01%	0.002%
18	3.751	839	843	845	rBV	243	194	0.02%	0.002%
19	3.895	877	888	932	rBV2	81512	274349	24.04%	3.142%
20	4.352	1013	1030	1058	rBV	183995	458900	40.22%	5.255%
21	4.596	1105	1106	1109	rBV2	388	240	0.02%	0.003%
22	4.696	1133	1137	1141	rBV2	196	162	0.01%	0.002%
23	4.722	1141	1145	1148	rVB3	439	325	0.03%	0.004%
24	4.744	1148	1152	1153	rBV2	318	243	0.02%	0.003%
25	4.809	1166	1172	1176	rBV2	317	332	0.03%	0.004%
26	4.850	1182	1185	1187	rBV2	315	146	0.01%	0.002%
27	5.050	1229	1247	1274	rBV2	443084	1140997	100.00%	13.067%
28	5.313	1327	1329	1331	rBV	401	160	0.01%	0.002%
29	5.342	1334	1338	1341	rVV3	520	348	0.03%	0.004%
30	5.400	1354	1356	1359	rBV2	307	145	0.01%	0.002%
31	5.452	1370	1372	1374	rBV3	291	154	0.01%	0.002%
32	5.506	1385	1389	1393	rVB	319	247	0.02%	0.003%
33	5.567	1405	1408	1411	rBV3	404	380	0.03%	0.004%
34	5.619	1412	1424	1452	rBV	345898	702962	61.61%	8.050%
35	5.915	1503	1516	1539	rBV4	64928	149487	13.10%	1.712%
36	6.072	1551	1565	1585	rBV	256906	519407	45.52%	5.948%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022173.D
 Acq On : 17 Sep 2021 09:56
 Operator : SY/MD
 Sample : M3764-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.374	1656	1659	1663	rVV2	435	248	0.02%	0.003%
38	6.419	1668	1673	1677	rVB3	414	401	0.04%	0.005%
39	6.542	1708	1711	1717	rBV3	427	359	0.03%	0.004%
40	6.625	1733	1737	1738	rBV	356	190	0.02%	0.002%
41	6.638	1738	1741	1742	rBV	490	279	0.02%	0.003%
42	6.722	1761	1767	1772	rVB3	381	408	0.04%	0.005%
43	6.796	1787	1790	1793	rBV3	183	158	0.01%	0.002%
44	6.989	1839	1850	1875	rVV	124910	231046	20.25%	2.646%
45	7.317	1940	1952	1972	rBV	522467	914968	80.19%	10.478%
46	7.625	2036	2048	2070	rBV	86461	154132	13.51%	1.765%
47	7.927	2139	2142	2144	rBV3	458	232	0.02%	0.003%
48	7.944	2145	2147	2155	rVB2	716	496	0.04%	0.006%
49	7.976	2155	2157	2160	rVB	343	169	0.01%	0.002%
50	7.998	2160	2164	2167	rBV2	200	147	0.01%	0.002%
51	8.021	2167	2171	2173	rVB3	311	228	0.02%	0.003%
52	8.095	2183	2194	2235	rBV2	268868	546967	47.94%	6.264%
53	8.362	2275	2277	2281	rBV4	483	328	0.03%	0.004%
54	8.439	2297	2301	2303	rBV2	726	397	0.03%	0.005%
55	8.474	2310	2312	2315	rBV	372	194	0.02%	0.002%
56	8.570	2340	2342	2346	rBV	209	158	0.01%	0.002%
57	8.628	2357	2360	2361	rBV2	365	207	0.02%	0.002%
58	8.641	2362	2364	2366	rVV2	412	150	0.01%	0.002%
59	8.718	2386	2388	2390	rBV2	299	144	0.01%	0.002%
60	8.773	2397	2405	2410	rBV	373	444	0.04%	0.005%
61	8.853	2418	2430	2466	rBV	518001	851748	74.65%	9.754%
62	9.149	2516	2522	2532	rVB7	1192	1706	0.15%	0.020%
63	9.204	2536	2539	2544	rVB3	429	343	0.03%	0.004%
64	9.326	2575	2577	2581	rBV	202	181	0.02%	0.002%
65	9.387	2594	2596	2599	rBV	367	191	0.02%	0.002%
66	9.413	2600	2604	2605	rBV	282	192	0.02%	0.002%
67	9.445	2612	2614	2621	rVB3	518	361	0.03%	0.004%
68	9.487	2622	2627	2631	rBV2	304	276	0.02%	0.003%
69	9.542	2641	2644	2646	rVB	386	200	0.02%	0.002%
70	9.558	2646	2649	2651	rBV2	378	333	0.03%	0.004%
71	9.603	2661	2663	2669	rVB	271	217	0.02%	0.002%
72	9.741	2700	2706	2709	rVB4	337	356	0.03%	0.004%
73	10.059	2802	2805	2807	rVV2	283	158	0.01%	0.002%
74	10.127	2820	2826	2830	rBV2	1625	1916	0.17%	0.022%
75	10.217	2843	2854	2878	rBV	324580	520943	45.66%	5.966%
76	10.358	2894	2898	2901	rBV2	538	453	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022173.D
 Acq On : 17 Sep 2021 09:56
 Operator : SY/MD
 Sample : M3764-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.468	2926	2932	2934	rBV3	189	201	0.02%	0.002%
78	10.599	2972	2973	2976	rVB3	554	186	0.02%	0.002%
79	10.648	2984	2988	2989	rBV2	245	148	0.01%	0.002%
80	10.702	3001	3005	3009	rBV2	304	208	0.02%	0.002%
81	10.770	3023	3026	3028	rBV3	427	227	0.02%	0.003%
82	10.808	3035	3038	3040	rBV	294	156	0.01%	0.002%
83	10.921	3069	3073	3081	rVB5	1914	2277	0.20%	0.026%
84	11.146	3136	3143	3145	rBV3	961	930	0.08%	0.011%
85	11.252	3164	3176	3196	rBV	488235	760798	66.68%	8.713%
86	11.490	3248	3250	3253	rVB2	332	163	0.01%	0.002%
87	11.506	3254	3255	3259	rVB	281	142	0.01%	0.002%
88	11.538	3263	3265	3267	rBV	331	180	0.02%	0.002%
89	11.564	3271	3273	3276	rVB2	400	193	0.02%	0.002%
90	11.625	3276	3292	3312	rBV	509906	798312	69.97%	9.142%
91	11.815	3349	3351	3353	rBV	445	240	0.02%	0.003%
92	11.930	3384	3387	3388	rBV	375	200	0.02%	0.002%
93	12.049	3421	3424	3426	rBV2	221	167	0.01%	0.002%
94	12.104	3439	3441	3443	rBV2	385	147	0.01%	0.002%
95	12.532	3572	3574	3578	rBV	338	237	0.02%	0.003%
96	12.602	3594	3596	3603	rBV3	469	444	0.04%	0.005%
97	12.693	3621	3624	3627	rVB	248	171	0.01%	0.002%
98	12.709	3627	3629	3631	rBV	254	143	0.01%	0.002%
99	12.828	3663	3666	3667	rBV	367	181	0.02%	0.002%
100	13.619	3910	3912	3915	rBV2	388	291	0.03%	0.003%




Sum of corrected areas: 8732218

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022173.D
Acq On : 17 Sep 2021 09:56
Operator : SY/MD
Sample : M3764-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

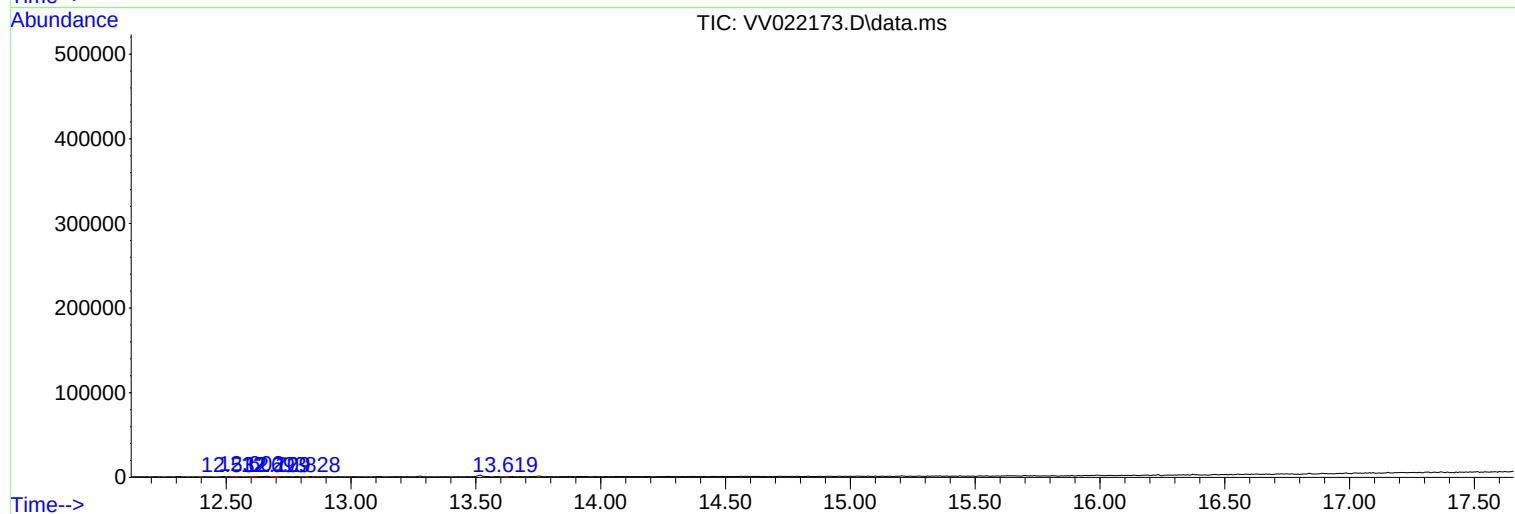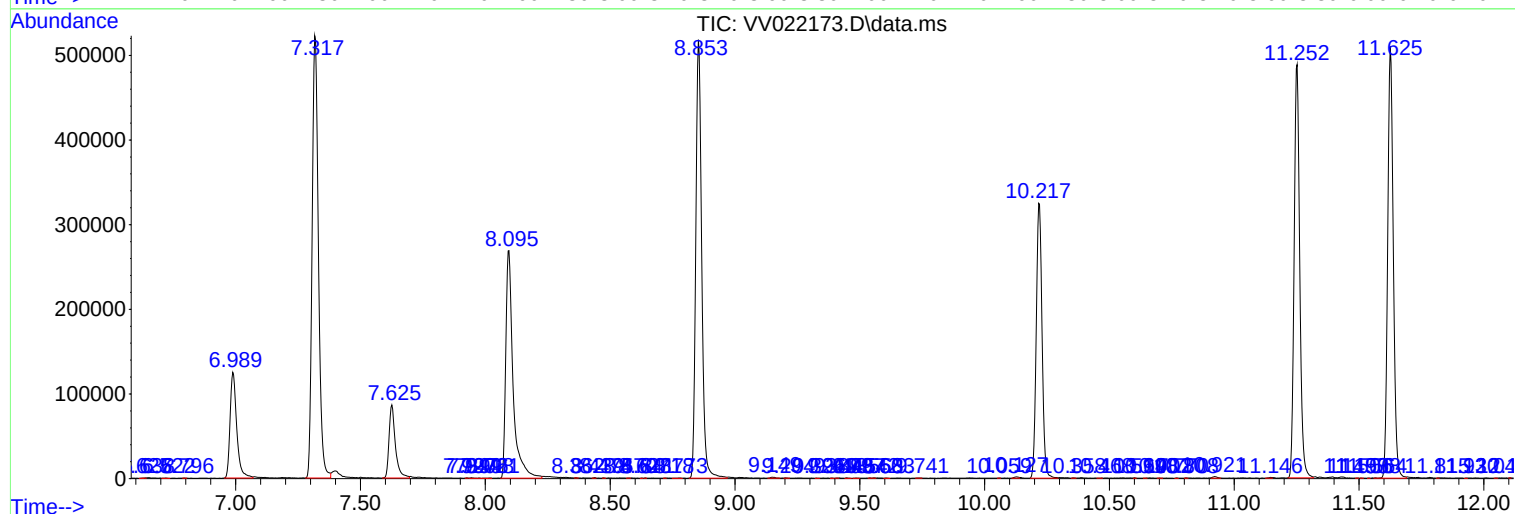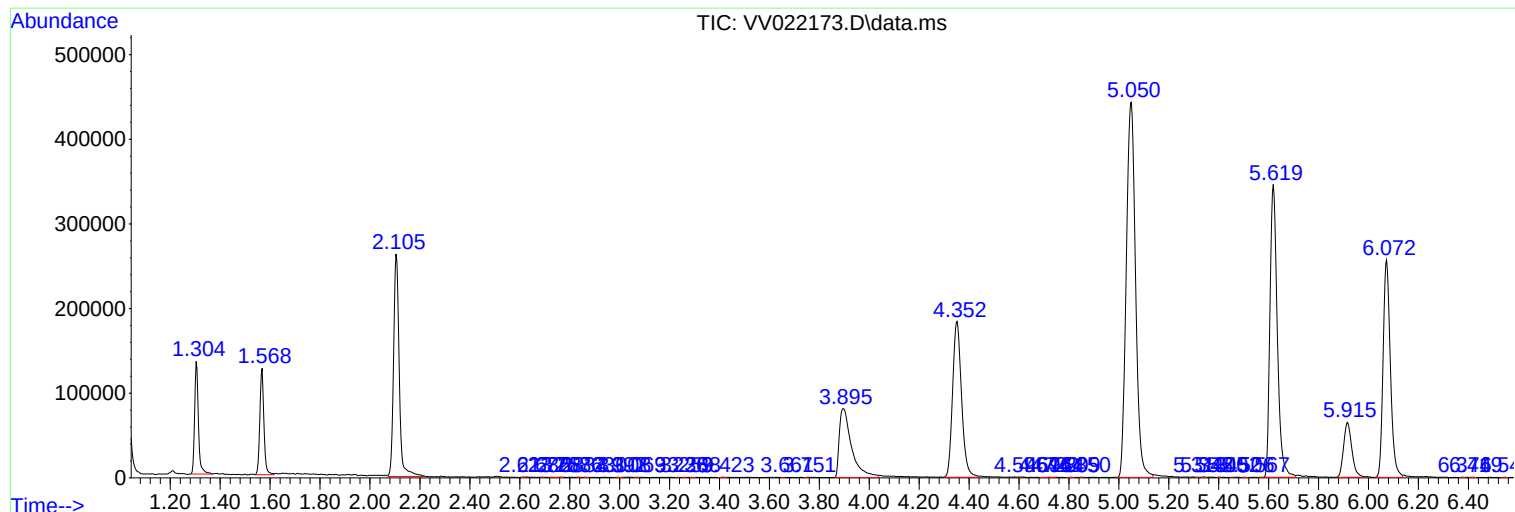

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022173.D
Acq On : 17 Sep 2021 09:56
Operator : SY/MD
Sample : M3764-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022173.D
Acq On : 17 Sep 2021 09:56
Operator : SY/MD
Sample : M3764-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
