

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022176.D
 Acq On : 17 Sep 2021 11:08
 Operator : SY/MD
 Sample : M3676-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022176.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rBV	126487	134130	12.34%	1.645%
2	1.564	156	163	175	rBV	123133	137645	12.67%	1.688%
3	2.105	321	331	355	rBV	243491	361814	33.29%	4.436%
4	2.597	482	484	488	rVB	431	258	0.02%	0.003%
5	2.728	522	525	526	rBV	356	226	0.02%	0.003%
6	2.899	574	578	580	rVB	309	175	0.02%	0.002%
7	2.950	591	594	597	rVB2	340	271	0.02%	0.003%
8	3.011	610	613	617	rBV2	228	154	0.01%	0.002%
9	3.047	620	624	629	rBV2	262	263	0.02%	0.003%
10	3.243	683	685	688	rVB	236	106	0.01%	0.001%
11	3.262	688	691	693	rBV2	247	136	0.01%	0.002%
12	3.387	728	730	733	rBV	218	179	0.02%	0.002%
13	3.442	741	747	751	rBV	289	286	0.03%	0.004%
14	3.465	752	754	762	rVB	296	226	0.02%	0.003%
15	3.503	762	766	768	rBV2	319	214	0.02%	0.003%
16	3.558	781	783	786	rVB2	412	144	0.01%	0.002%
17	3.622	800	803	807	rBV2	170	120	0.01%	0.001%
18	3.892	877	887	920	rBV2	81013	250260	23.03%	3.068%
19	4.352	1014	1030	1057	rBV	172607	428820	39.46%	5.258%
20	4.603	1106	1108	1112	rVB	278	140	0.01%	0.002%
21	4.625	1112	1115	1118	rBV3	261	177	0.02%	0.002%
22	4.651	1118	1123	1124	rBV2	459	301	0.03%	0.004%
23	4.680	1130	1132	1133	rBV	240	118	0.01%	0.001%
24	4.731	1145	1148	1149	rBV	237	118	0.01%	0.001%
25	4.760	1154	1157	1160	rBV2	159	131	0.01%	0.002%
26	4.799	1164	1169	1173	rBV2	258	277	0.03%	0.003%
27	4.822	1173	1176	1178	rBV2	225	154	0.01%	0.002%
28	4.918	1204	1206	1209	rBV	208	158	0.01%	0.002%
29	5.047	1229	1246	1276	rBV2	429513	1086753	100.00%	13.325%
30	5.413	1358	1360	1362	rBV2	210	123	0.01%	0.002%
31	5.465	1372	1376	1379	rVB3	360	257	0.02%	0.003%
32	5.490	1379	1384	1388	rBV3	482	515	0.05%	0.006%
33	5.619	1410	1424	1462	rBV	328875	664837	61.18%	8.152%
34	5.912	1502	1515	1543	rBV5	46258	114107	10.50%	1.399%
35	6.072	1551	1565	1587	rBV	241818	497934	45.82%	6.105%
36	6.284	1629	1631	1635	rVB2	469	225	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V091721\
 Data File : VV022176.D
 Acq On : 17 Sep 2021 11:08
 Operator : SY/MD
 Sample : M3676-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.339	1644	1648	1651	rBV2	320	251	0.02%	0.003%
38	6.352	1651	1652	1654	rVV2	389	140	0.01%	0.002%
39	6.375	1657	1659	1662	rBV3	379	214	0.02%	0.003%
40	6.391	1662	1664	1668	rVV3	442	264	0.02%	0.003%
41	6.429	1673	1676	1678	rBV2	273	127	0.01%	0.002%
42	6.452	1681	1683	1686	rBV	287	114	0.01%	0.001%
43	6.526	1704	1706	1709	rBV2	230	114	0.01%	0.001%
44	6.580	1721	1723	1731	rVB3	429	282	0.03%	0.003%
45	6.616	1731	1734	1737	rVB	251	140	0.01%	0.002%
46	6.635	1737	1740	1743	rBV2	407	292	0.03%	0.004%
47	6.915	1824	1827	1828	rBV	384	179	0.02%	0.002%
48	6.989	1839	1850	1871	rBV	114574	214912	19.78%	2.635%
49	7.239	1926	1928	1930	rBV2	317	183	0.02%	0.002%
50	7.317	1940	1952	1972	rBV	491026	859831	79.12%	10.543%
51	7.625	2037	2048	2068	rBV	78775	140963	12.97%	1.728%
52	7.751	2084	2087	2090	rBV2	547	370	0.03%	0.005%
53	7.789	2097	2099	2104	rVB4	295	217	0.02%	0.003%
54	7.947	2136	2148	2156	rBV4	1881	3181	0.29%	0.039%
55	8.091	2183	2193	2234	rBV2	258243	518839	47.74%	6.362%
56	8.378	2279	2282	2285	rBV3	553	366	0.03%	0.004%
57	8.468	2307	2310	2313	rBV3	425	372	0.03%	0.005%
58	8.609	2350	2354	2355	rBV	410	249	0.02%	0.003%
59	8.645	2362	2365	2368	rBV2	208	149	0.01%	0.002%
60	8.741	2392	2395	2398	rBV3	221	179	0.02%	0.002%
61	8.805	2411	2415	2416	rBV2	503	212	0.02%	0.003%
62	8.854	2419	2430	2459	rBV	485414	793299	73.00%	9.727%
63	9.207	2537	2540	2544	rBV	381	222	0.02%	0.003%
64	9.233	2545	2548	2551	rVV2	339	163	0.01%	0.002%
65	9.336	2576	2580	2581	rBV	242	115	0.01%	0.001%
66	9.419	2602	2606	2608	rBV2	211	136	0.01%	0.002%
67	9.632	2670	2672	2674	rBV2	196	120	0.01%	0.001%
68	9.770	2713	2715	2717	rBV	211	121	0.01%	0.001%
69	9.853	2740	2741	2744	rVB	357	162	0.01%	0.002%
70	9.873	2744	2747	2748	rBV	343	188	0.02%	0.002%
71	9.921	2759	2762	2763	rBV	227	114	0.01%	0.001%
72	9.950	2769	2771	2772	rBV	240	117	0.01%	0.001%
73	10.085	2811	2813	2816	rVB2	164	103	0.01%	0.001%
74	10.127	2816	2826	2836	rBV4	1667	2591	0.24%	0.032%
75	10.217	2843	2854	2868	rBV	313488	494863	45.54%	6.068%
76	10.345	2891	2894	2900	rVV3	471	414	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022176.D
 Acq On : 17 Sep 2021 11:08
 Operator : SY/MD
 Sample : M3676-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.384	2900	2906	2915	rVB6	2049	3037	0.28%	0.037%
78	10.513	2944	2946	2949	rVB	216	121	0.01%	0.001%
79	10.545	2954	2956	2958	rBV2	347	164	0.02%	0.002%
80	10.657	2989	2991	2993	rVB	276	114	0.01%	0.001%
81	10.751	3014	3020	3023	rBV2	403	471	0.04%	0.006%
82	10.812	3036	3039	3041	rBV2	377	225	0.02%	0.003%
83	10.892	3063	3064	3066	rBV2	353	163	0.01%	0.002%
84	11.030	3101	3107	3109	rBV3	407	267	0.02%	0.003%
85	11.133	3137	3139	3140	rBV	321	123	0.01%	0.002%
86	11.201	3155	3160	3164	rVB2	374	390	0.04%	0.005%
87	11.252	3164	3176	3204	rBV	444481	695120	63.96%	8.523%
88	11.490	3248	3250	3255	rVB	377	245	0.02%	0.003%
89	11.625	3280	3292	3316	rBV	471548	736519	67.77%	9.031%
90	11.882	3369	3372	3374	rBV	442	291	0.03%	0.004%
91	12.033	3417	3419	3421	rBV3	284	161	0.01%	0.002%
92	12.172	3458	3462	3465	rBV2	374	322	0.03%	0.004%
93	12.355	3515	3519	3520	rBV	342	254	0.02%	0.003%
94	12.879	3681	3682	3685	rBV	228	126	0.01%	0.002%
95	12.959	3704	3707	3711	rBV2	309	220	0.02%	0.003%
96	13.004	3719	3721	3726	rVB2	256	135	0.01%	0.002%
97	13.300	3811	3813	3815	rBV	286	125	0.01%	0.002%
98	13.410	3845	3847	3850	rVB2	337	181	0.02%	0.002%
99	14.040	4041	4043	4046	rBV	455	237	0.02%	0.003%
100	14.056	4046	4048	4051	rVV2	392	163	0.01%	0.002%




Sum of corrected areas: 8155794

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022176.D
Acq On : 17 Sep 2021 11:08
Operator : SY/MD
Sample : M3676-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CB5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

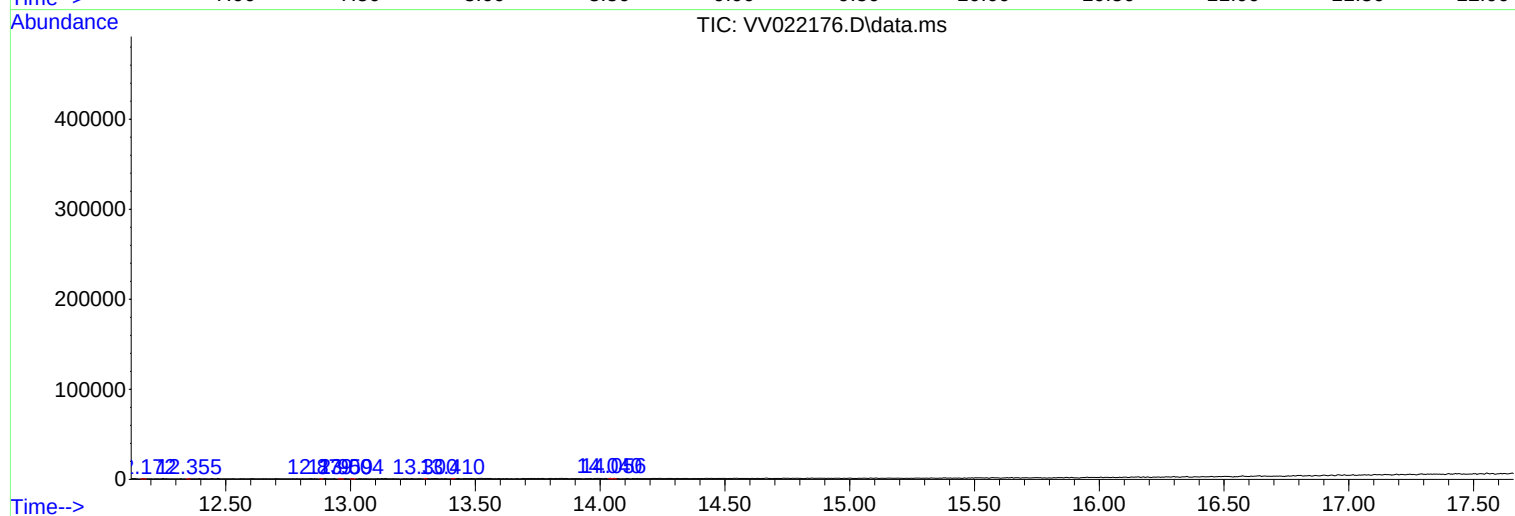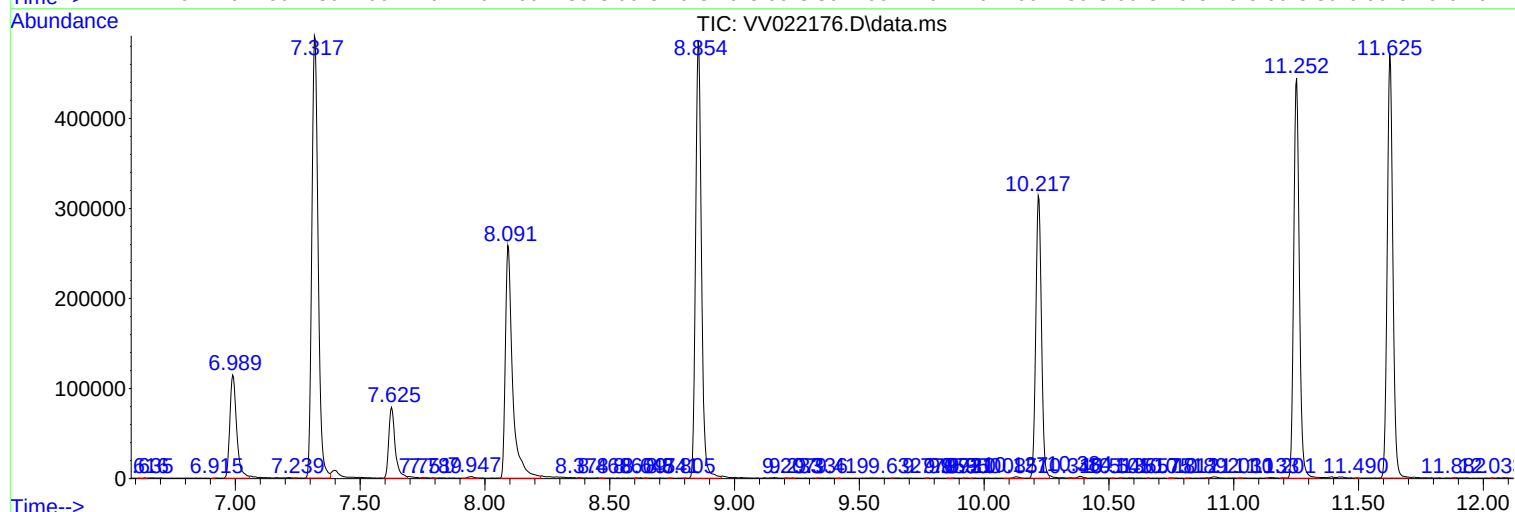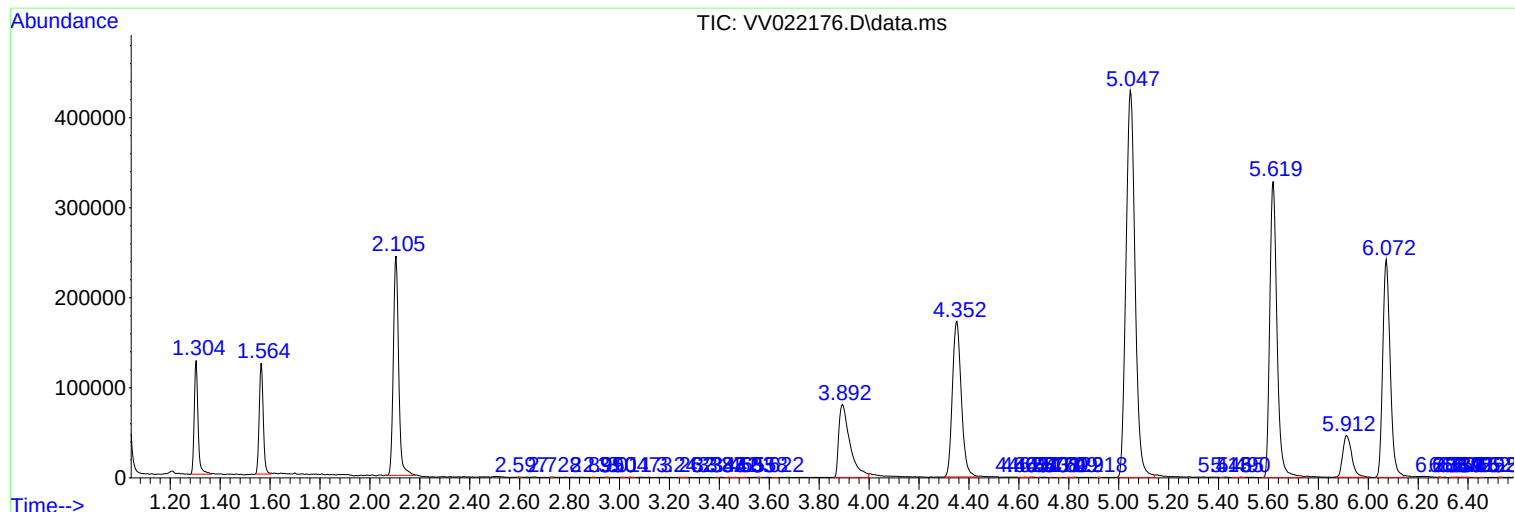

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022176.D
Acq On : 17 Sep 2021 11:08
Operator : SY/MD
Sample : M3676-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CB5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022176.D
Acq On : 17 Sep 2021 11:08
Operator : SY/MD
Sample : M3676-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CB5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
