

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022182.D
 Acq On : 17 Sep 2021 13:33
 Operator : SY/MD
 Sample : M3778-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E4586

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022182.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rBV	117726	122689	1.74%	0.766%
2	1.565	156	163	177	rBV	116068	131819	1.86%	0.823%
3	2.105	322	331	344	rBV	238466	339747	4.81%	2.121%
4	2.510	450	457	471	rVB4	1922	3106	0.04%	0.019%
5	2.767	528	537	548	rVB3	5727	9924	0.14%	0.062%
6	2.812	548	551	554	rBV2	383	219	0.00%	0.001%
7	3.089	633	637	639	rVB2	294	163	0.00%	0.001%
8	3.150	653	656	662	rBV3	253	254	0.00%	0.002%
9	3.191	668	669	670	rBV	242	85	0.00%	0.001%
10	3.220	674	678	683	rVB2	423	447	0.01%	0.003%
11	3.275	693	695	699	rVB2	365	171	0.00%	0.001%
12	3.304	703	704	705	rBV	275	67	0.00%	0.000%
13	3.314	705	707	712	rVB2	399	354	0.01%	0.002%
14	3.500	763	765	770	rVB2	606	416	0.01%	0.003%
15	3.526	770	773	774	rBV2	324	215	0.00%	0.001%
16	3.542	776	778	779	rVV	292	115	0.00%	0.001%
17	3.555	780	782	785	rVB2	275	151	0.00%	0.001%
18	3.632	803	806	808	rBV	431	217	0.00%	0.001%
19	3.777	850	851	854	rVB	479	179	0.00%	0.001%
20	3.793	854	856	857	rBV	174	83	0.00%	0.001%
21	3.905	878	891	930	rBV4	106480	365740	5.17%	2.283%
22	4.352	1012	1030	1060	rBV	171821	430958	6.10%	2.690%
23	4.709	1139	1141	1146	rBV2	348	282	0.00%	0.002%
24	4.828	1175	1178	1180	rBV2	235	139	0.00%	0.001%
25	4.841	1180	1182	1184	rVV	226	132	0.00%	0.001%
26	4.883	1192	1195	1197	rBV2	514	327	0.00%	0.002%
27	4.918	1204	1206	1208	rVB	332	128	0.00%	0.001%
28	4.934	1208	1211	1212	rBV	258	120	0.00%	0.001%
29	4.966	1218	1221	1222	rBV	322	169	0.00%	0.001%
30	4.989	1225	1228	1230	rBV2	185	102	0.00%	0.001%
31	5.047	1230	1246	1271	rBV2	427382	1080703	15.29%	6.746%
32	5.359	1339	1343	1346	rVB2	558	343	0.00%	0.002%
33	5.503	1387	1388	1389	rVB	381	74	0.00%	0.000%
34	5.619	1411	1424	1450	rBV	331999	674746	9.55%	4.212%
35	5.915	1501	1516	1551	rBV2	304975	629465	8.90%	3.929%
36	6.072	1552	1565	1595	rVB	242144	497229	7.03%	3.104%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW091721\
 Data File : VW022182.D
 Acq On : 17 Sep 2021 13:33
 Operator : SY/MD
 Sample : M3778-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E4586

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.368	1655	1657	1659	rBV	367	150	0.00%	0.001%
38	6.497	1696	1697	1698	rBV	184	48	0.00%	0.000%
39	6.744	1771	1774	1775	rBV2	306	147	0.00%	0.001%
40	6.805	1788	1793	1795	rVB2	367	287	0.00%	0.002%
41	6.818	1795	1797	1799	rBV2	308	134	0.00%	0.001%
42	6.857	1807	1809	1811	rBV2	365	133	0.00%	0.001%
43	6.892	1818	1820	1823	rVB	321	132	0.00%	0.001%
44	6.908	1823	1825	1828	rBV2	173	137	0.00%	0.001%
45	6.947	1832	1837	1838	rBV	285	207	0.00%	0.001%
46	6.989	1839	1850	1873	rBV	124531	229851	3.25%	1.435%
47	7.317	1940	1952	1972	rBV	494650	865741	12.25%	5.404%
48	7.561	2026	2028	2030	rBV2	514	279	0.00%	0.002%
49	7.625	2038	2048	2070	rBV	84517	149934	2.12%	0.936%
50	7.780	2093	2096	2098	rBV3	439	271	0.00%	0.002%
51	7.831	2110	2112	2114	rVB2	444	151	0.00%	0.001%
52	7.979	2143	2158	2184	rBV	4275432	7068712	100.00%	44.124%
53	8.092	2185	2193	2227	rVB	285103	556007	7.87%	3.471%
54	8.786	2405	2409	2412	rBV3	423	370	0.01%	0.002%
55	8.854	2419	2430	2452	rBV	503268	812379	11.49%	5.071%
56	9.146	2518	2521	2522	rBV	560	318	0.00%	0.002%
57	9.301	2566	2569	2572	rBV	276	157	0.00%	0.001%
58	9.400	2599	2600	2605	rBV3	446	308	0.00%	0.002%
59	9.510	2631	2634	2639	rBV2	347	328	0.00%	0.002%
60	9.709	2691	2696	2698	rBV2	272	267	0.00%	0.002%
61	9.741	2704	2706	2707	rBV	283	104	0.00%	0.001%
62	9.847	2737	2739	2744	rBV3	302	274	0.00%	0.002%
63	9.931	2763	2765	2768	rBV	348	210	0.00%	0.001%
64	10.217	2842	2854	2874	rBV	333156	523768	7.41%	3.269%
65	10.384	2901	2906	2915	rVB4	3011	4067	0.06%	0.025%
66	10.924	3067	3074	3080	rBV5	1516	2353	0.03%	0.015%
67	11.252	3164	3176	3196	rBV	464901	732027	10.36%	4.569%
68	11.535	3255	3264	3279	rBV4	11232	22678	0.32%	0.142%
69	11.625	3281	3292	3317	rVB	475081	755008	10.68%	4.713%
70	12.053	3424	3425	3428	rVB	489	151	0.00%	0.001%
71	12.384	3526	3528	3531	rBV2	329	225	0.00%	0.001%
72	12.519	3568	3570	3575	rVB3	425	285	0.00%	0.002%
73	12.715	3629	3631	3634	rBV	288	146	0.00%	0.001%
74	12.783	3650	3652	3653	rBV	257	84	0.00%	0.001%
75	12.944	3700	3702	3707	rBV3	523	244	0.00%	0.002%
76	12.998	3715	3719	3722	rBV2	432	306	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022182.D
Acq On : 17 Sep 2021 13:33
Operator : SY/MD
Sample : M3778-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E4586

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Title : VOC Analysis

77	13.776	3959	3961	3962	rBV	377	130	0.00%	0.001%
78	14.194	4088	4091	4094	rBV	465	353	0.00%	0.002%




Sum of corrected areas: 16019939

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022182.D
Acq On : 17 Sep 2021 13:33
Operator : SY/MD
Sample : M3778-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E4586

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

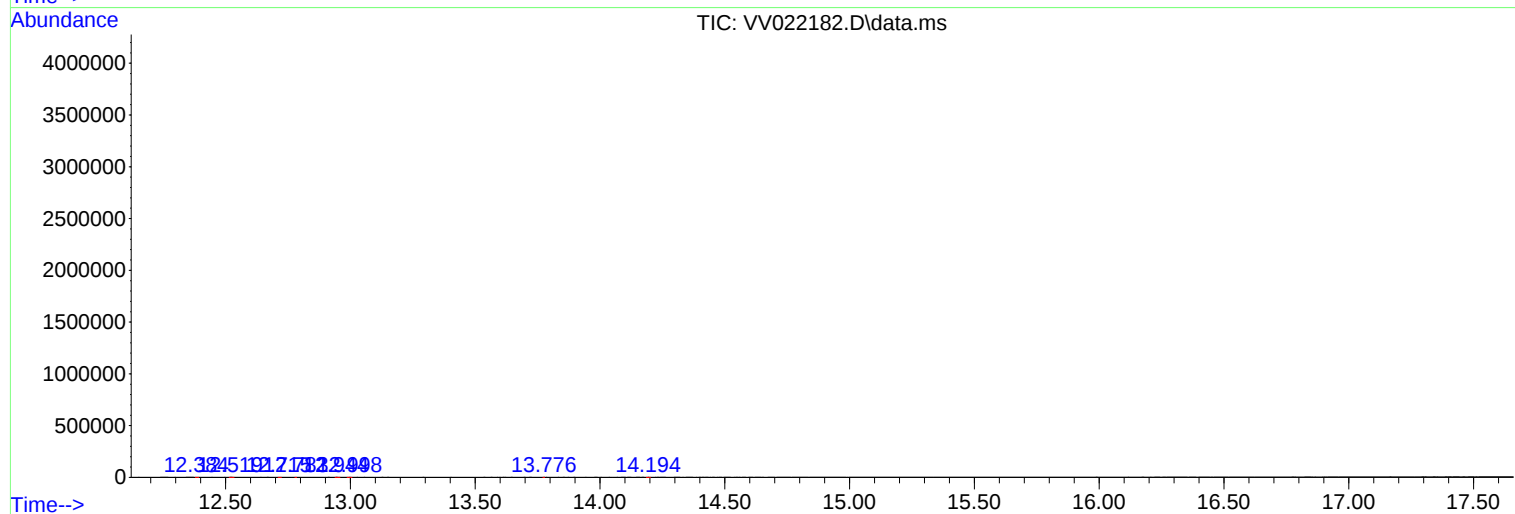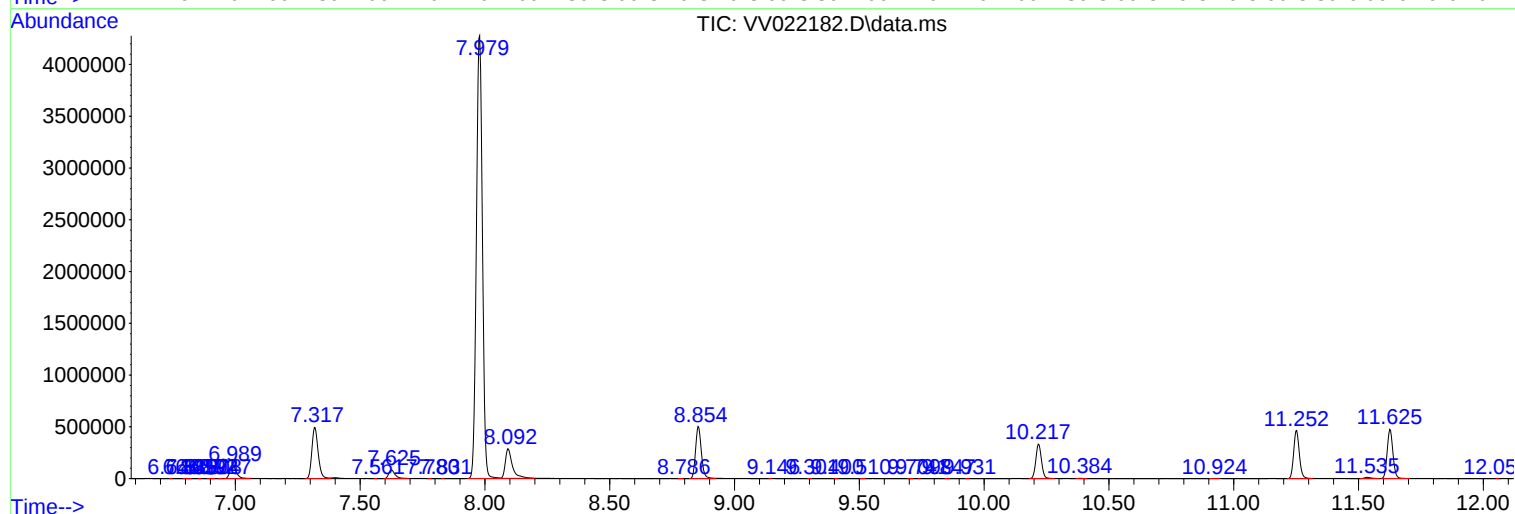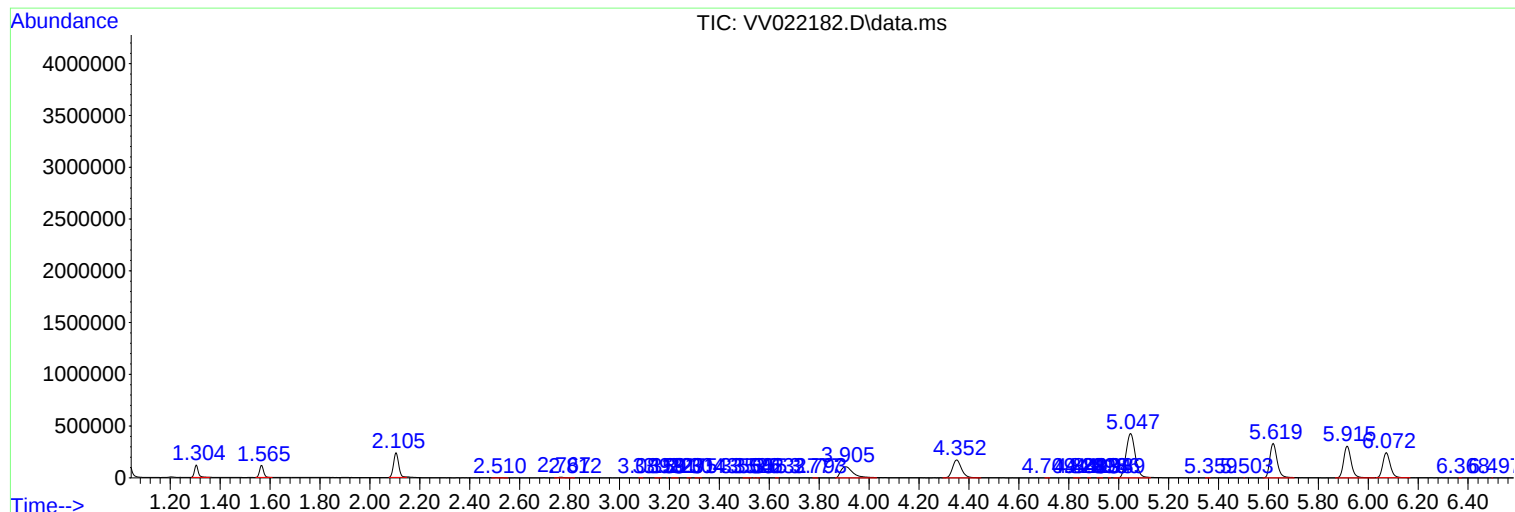

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022182.D
Acq On : 17 Sep 2021 13:33
Operator : SY/MD
Sample : M3778-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E4586

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022182.D
Acq On : 17 Sep 2021 13:33
Operator : SY/MD
Sample : M3778-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E4586

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
