

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022187.D
 Acq On : 17 Sep 2021 15:52
 Operator : SY/MD
 Sample : M3676-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022187.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	111028	115682	10.80%	1.407%
2	1.568	157	164	179	rVB	112056	124545	11.63%	1.515%
3	2.108	322	332	349	rBV	227899	337254	31.49%	4.102%
4	2.626	484	493	494	rBV4	800	933	0.09%	0.011%
5	2.661	501	504	507	rBV3	754	645	0.06%	0.008%
6	2.870	565	569	572	rBV2	224	177	0.02%	0.002%
7	2.889	572	575	579	rVV3	365	273	0.03%	0.003%
8	2.973	597	601	604	rBV2	289	271	0.03%	0.003%
9	3.027	614	618	620	rBV2	204	160	0.01%	0.002%
10	3.040	620	622	626	rVB2	349	211	0.02%	0.003%
11	3.072	629	632	635	rVB	264	166	0.02%	0.002%
12	3.105	636	642	644	rBV	382	254	0.02%	0.003%
13	3.314	702	707	708	rBV2	246	155	0.01%	0.002%
14	3.519	768	771	775	rVB3	306	238	0.02%	0.003%
15	3.651	808	812	815	rBV	252	177	0.02%	0.002%
16	3.690	821	824	826	rVB2	340	199	0.02%	0.002%
17	3.712	826	831	834	rBV2	248	260	0.02%	0.003%
18	3.899	878	889	926	rBV2	81634	275693	25.74%	3.353%
19	4.352	1015	1030	1054	rBV	171787	427076	39.87%	5.194%
20	4.548	1088	1091	1092	rBV3	302	217	0.02%	0.003%
21	4.674	1127	1130	1133	rBV2	353	243	0.02%	0.003%
22	4.754	1153	1155	1159	rVB	486	261	0.02%	0.003%
23	4.780	1159	1163	1164	rBV	255	150	0.01%	0.002%
24	4.838	1179	1181	1184	rBV2	307	152	0.01%	0.002%
25	4.966	1219	1221	1222	rBV2	349	146	0.01%	0.002%
26	5.050	1227	1247	1276	rBV2	422667	1071093	100.00%	13.027%
27	5.326	1329	1333	1335	rBV2	349	190	0.02%	0.002%
28	5.375	1345	1348	1353	rVB4	616	442	0.04%	0.005%
29	5.426	1360	1364	1367	rBV4	395	313	0.03%	0.004%
30	5.474	1376	1379	1384	rBV2	387	308	0.03%	0.004%
31	5.497	1384	1386	1389	rVV	340	226	0.02%	0.003%
32	5.619	1411	1424	1447	rBV	321333	651214	60.80%	7.921%
33	5.912	1503	1515	1538	rVB6	30357	73273	6.84%	0.891%
34	6.005	1542	1544	1547	rBV2	254	153	0.01%	0.002%
35	6.072	1551	1565	1586	rBV	236547	488224	45.58%	5.938%
36	6.214	1604	1609	1611	rBV3	1209	1055	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022187.D
 Acq On : 17 Sep 2021 15:52
 Operator : SY/MD
 Sample : M3676-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.436	1673	1678	1685	rBV2	218	269	0.03%	0.003%
38	6.468	1687	1688	1690	rBV2	481	189	0.02%	0.002%
39	6.487	1690	1694	1698	rVB2	301	206	0.02%	0.003%
40	6.510	1698	1701	1706	rBV3	390	254	0.02%	0.003%
41	6.542	1707	1711	1714	rVB4	503	354	0.03%	0.004%
42	6.580	1720	1723	1727	rBV2	483	299	0.03%	0.004%
43	6.712	1762	1764	1766	rBV	387	215	0.02%	0.003%
44	6.789	1784	1788	1791	rBV3	324	191	0.02%	0.002%
45	6.812	1792	1795	1798	rVB2	278	179	0.02%	0.002%
46	6.863	1806	1811	1815	rBV2	384	341	0.03%	0.004%
47	6.992	1839	1851	1871	rBV	120487	223794	20.89%	2.722%
48	7.175	1906	1908	1912	rBV4	443	392	0.04%	0.005%
49	7.259	1932	1934	1937	rVB3	397	199	0.02%	0.002%
50	7.320	1940	1953	1972	rBV	488160	849647	79.33%	10.334%
51	7.625	2039	2048	2079	rBV	80539	145059	13.54%	1.764%
52	7.947	2137	2148	2150	rBV3	1034	1497	0.14%	0.018%
53	7.982	2150	2159	2169	rVB3	9614	16434	1.53%	0.200%
54	8.092	2178	2193	2236	rBV2	316889	648967	60.59%	7.893%
55	8.410	2289	2292	2296	rBV2	668	478	0.04%	0.006%
56	8.439	2299	2301	2303	rBV3	483	207	0.02%	0.003%
57	8.571	2338	2342	2346	rBV4	547	549	0.05%	0.007%
58	8.645	2362	2365	2366	rBV2	348	169	0.02%	0.002%
59	8.786	2400	2409	2416	rVB3	307	530	0.05%	0.006%
60	8.857	2419	2431	2458	rBV	481369	786589	73.44%	9.567%
61	9.066	2494	2496	2498	rBV2	258	162	0.02%	0.002%
62	9.101	2504	2507	2508	rBV	259	169	0.02%	0.002%
63	9.230	2543	2547	2549	rBV	325	194	0.02%	0.002%
64	9.262	2555	2557	2560	rVB3	329	194	0.02%	0.002%
65	9.326	2574	2577	2581	rVB2	387	229	0.02%	0.003%
66	9.342	2581	2582	2586	rBV2	372	244	0.02%	0.003%
67	9.487	2624	2627	2631	rVV2	465	335	0.03%	0.004%
68	9.548	2642	2646	2648	rBV3	447	327	0.03%	0.004%
69	9.747	2703	2708	2713	rVB2	335	369	0.03%	0.004%
70	9.773	2713	2716	2719	rBV2	448	251	0.02%	0.003%
71	9.947	2767	2770	2778	rBV2	354	352	0.03%	0.004%
72	10.030	2791	2796	2798	rVB	294	205	0.02%	0.002%
73	10.053	2798	2803	2806	rBV2	267	213	0.02%	0.003%
74	10.072	2806	2809	2810	rBV2	310	190	0.02%	0.002%
75	10.098	2814	2817	2819	rBV2	270	174	0.02%	0.002%
76	10.130	2819	2827	2839	rVB5	2168	3607	0.34%	0.044%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022187.D
 Acq On : 17 Sep 2021 15:52
 Operator : SY/MD
 Sample : M3676-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.220	2843	2855	2871	rBV	317975	504612	47.11%	6.137%
78	10.429	2916	2920	2924	rVB	350	227	0.02%	0.003%
79	10.490	2935	2939	2942	rVB	419	338	0.03%	0.004%
80	10.516	2942	2947	2951	rBV3	693	599	0.06%	0.007%
81	10.554	2957	2959	2962	rBV3	359	178	0.02%	0.002%
82	10.661	2989	2992	2995	rVB2	357	194	0.02%	0.002%
83	10.918	3063	3072	3074	rBV3	1776	1810	0.17%	0.022%
84	10.995	3090	3096	3099	rBV3	274	255	0.02%	0.003%
85	11.030	3104	3107	3109	rVV2	339	198	0.02%	0.002%
86	11.085	3122	3124	3127	rBV2	274	180	0.02%	0.002%
87	11.146	3140	3143	3145	rBV2	713	424	0.04%	0.005%
88	11.252	3163	3176	3195	rBV	451557	709062	66.20%	8.624%
89	11.384	3214	3217	3219	rBV2	884	636	0.06%	0.008%
90	11.490	3248	3250	3254	rVB4	393	233	0.02%	0.003%
91	11.542	3262	3266	3274	rBV6	851	1059	0.10%	0.013%
92	11.625	3280	3292	3314	rBV	464741	742581	69.33%	9.032%
93	11.847	3359	3361	3363	rBV2	571	287	0.03%	0.003%
94	12.095	3435	3438	3443	rVB3	987	968	0.09%	0.012%
95	12.387	3527	3529	3533	rBV	548	230	0.02%	0.003%
96	12.529	3571	3573	3576	rBV	249	165	0.02%	0.002%
97	12.603	3591	3596	3602	rBV4	628	637	0.06%	0.008%
98	12.738	3634	3638	3640	rBV	455	292	0.03%	0.004%
99	13.220	3785	3788	3790	rBV	353	191	0.02%	0.002%
100	13.525	3881	3883	3887	rBV2	301	229	0.02%	0.003%




Sum of corrected areas: 8221837

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022187.D
Acq On : 17 Sep 2021 15:52
Operator : SY/MD
Sample : M3676-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

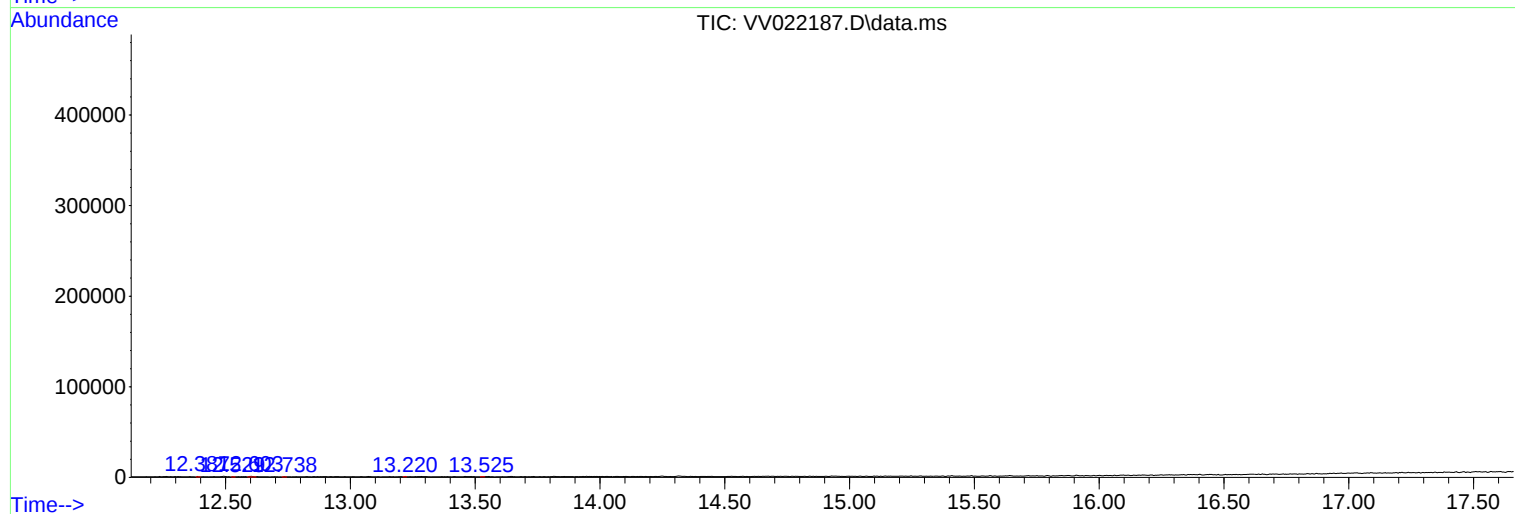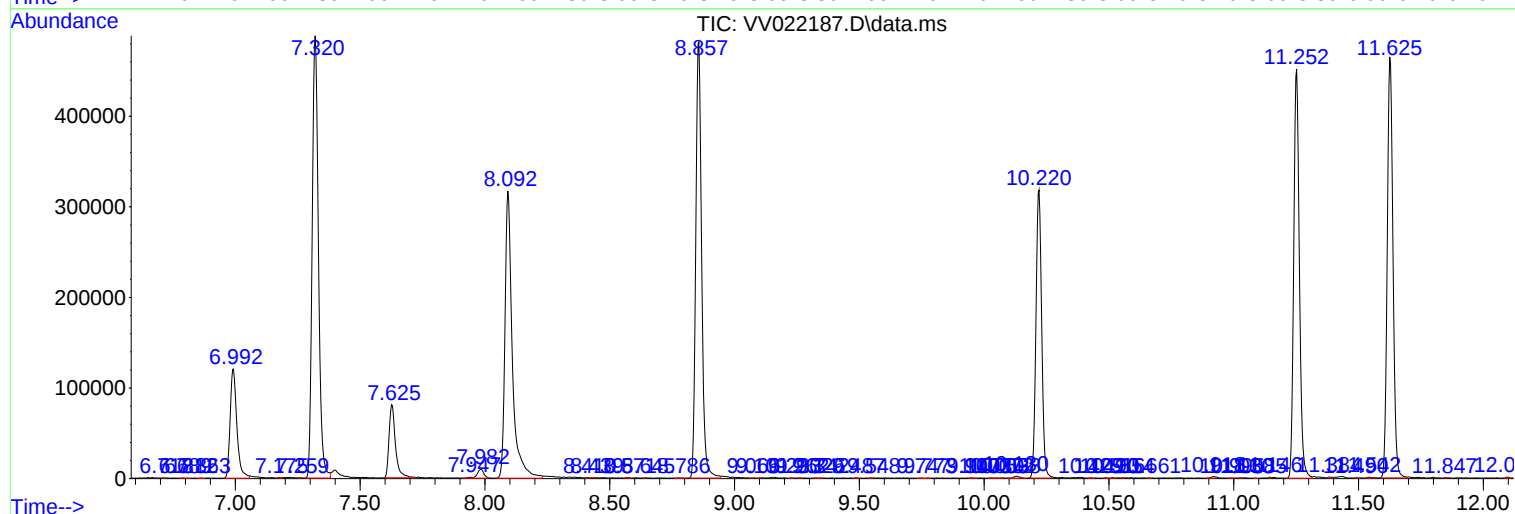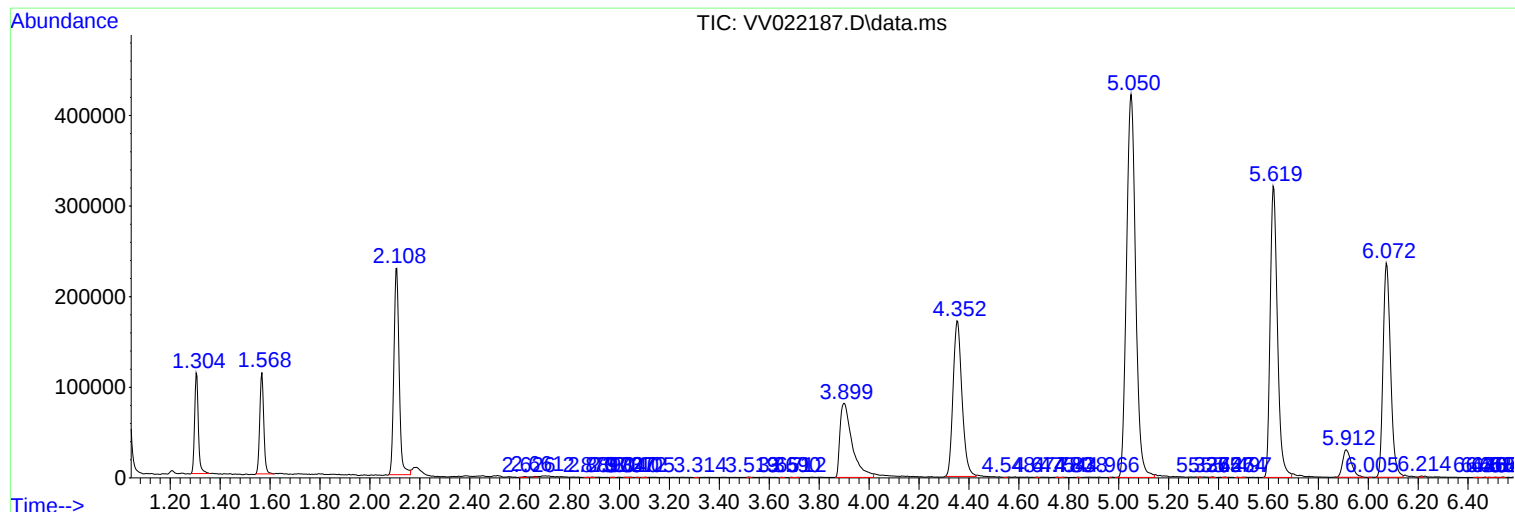

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022187.D
Acq On : 17 Sep 2021 15:52
Operator : SY/MD
Sample : M3676-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022187.D
Acq On : 17 Sep 2021 15:52
Operator : SY/MD
Sample : M3676-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
