

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022194.D
 Acq On : 17 Sep 2021 18:41
 Operator : SY/MD
 Sample : M3676-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022194.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	93	rBV	107428	109723	10.44%	1.200%
2	1.564	156	163	174	rBV	109632	125009	11.89%	1.367%
3	2.105	322	331	370	rVB2	240650	395521	37.62%	4.326%
4	2.709	514	519	521	rBV3	460	353	0.03%	0.004%
5	2.789	542	544	547	rVB2	348	169	0.02%	0.002%
6	2.854	561	564	566	rBV2	312	171	0.02%	0.002%
7	2.969	598	600	603	rVB3	464	226	0.02%	0.002%
8	3.066	628	630	634	rVB2	467	188	0.02%	0.002%
9	3.108	637	643	645	rBV3	333	227	0.02%	0.002%
10	3.191	661	669	684	rVB3	4738	9752	0.93%	0.107%
11	3.294	698	701	704	rVV3	323	191	0.02%	0.002%
12	3.641	803	809	810	rBV2	208	183	0.02%	0.002%
13	3.748	837	842	846	rVB2	243	190	0.02%	0.002%
14	3.776	848	851	854	rBV2	381	296	0.03%	0.003%
15	3.815	861	863	867	rBV2	265	168	0.02%	0.002%
16	3.854	873	875	879	rVB2	316	187	0.02%	0.002%
17	3.905	879	891	925	rBV2	96182	345910	32.90%	3.783%
18	4.352	1013	1030	1056	rBV	167555	418383	39.79%	4.576%
19	4.670	1127	1129	1133	rVB4	419	221	0.02%	0.002%
20	4.831	1176	1179	1182	rBV2	396	256	0.02%	0.003%
21	4.876	1190	1193	1197	rBV	245	179	0.02%	0.002%
22	5.050	1228	1247	1275	rBV2	412874	1051410	100.00%	11.499%
23	5.272	1313	1316	1318	rBV2	399	205	0.02%	0.002%
24	5.410	1353	1359	1360	rBV2	335	229	0.02%	0.003%
25	5.452	1370	1372	1376	rBV	600	333	0.03%	0.004%
26	5.506	1387	1389	1393	rVB3	382	196	0.02%	0.002%
27	5.535	1393	1398	1400	rBV	273	161	0.02%	0.002%
28	5.619	1412	1424	1451	rBV	329800	663886	63.14%	7.261%
29	5.915	1502	1516	1548	rBV	528989	1051246	99.98%	11.497%
30	6.072	1553	1565	1594	rVB	239099	486030	46.23%	5.316%
31	6.307	1637	1638	1641	rBV2	352	173	0.02%	0.002%
32	6.445	1677	1681	1685	rVB2	498	297	0.03%	0.003%
33	6.622	1733	1736	1738	rVB2	382	175	0.02%	0.002%
34	6.645	1739	1743	1745	rBV2	614	442	0.04%	0.005%
35	6.773	1780	1783	1786	rBV3	315	190	0.02%	0.002%
36	6.815	1791	1796	1802	rBV2	259	298	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022194.D
 Acq On : 17 Sep 2021 18:41
 Operator : SY/MD
 Sample : M3676-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.989	1840	1850	1879	rBV	115075	216086	20.55%	2.363%
38	7.255	1931	1933	1936	rBV2	319	185	0.02%	0.002%
39	7.320	1940	1953	1971	rBV	460924	817054	77.71%	8.936%
40	7.590	2031	2037	2038	rBV4	433	436	0.04%	0.005%
41	7.625	2039	2048	2074	rVV	78124	139340	13.25%	1.524%
42	7.847	2113	2117	2118	rBV	573	316	0.03%	0.003%
43	7.902	2132	2134	2136	rVB	496	168	0.02%	0.002%
44	7.921	2137	2140	2142	rBV	245	170	0.02%	0.002%
45	7.950	2142	2149	2151	rBV5	1098	1320	0.13%	0.014%
46	7.982	2153	2159	2169	rVB6	4464	7024	0.67%	0.077%
47	8.021	2169	2171	2175	rVB2	402	204	0.02%	0.002%
48	8.095	2184	2194	2230	rBV2	251833	514351	48.92%	5.625%
49	8.371	2271	2280	2295	rVB7	4924	10055	0.96%	0.110%
50	8.490	2315	2317	2320	rVB2	325	160	0.02%	0.002%
51	8.506	2320	2322	2325	rBV2	410	272	0.03%	0.003%
52	8.551	2334	2336	2338	rBV	381	202	0.02%	0.002%
53	8.603	2349	2352	2354	rBV	397	179	0.02%	0.002%
54	8.616	2354	2356	2360	rVB2	435	229	0.02%	0.003%
55	8.635	2360	2362	2369	rBV3	465	445	0.04%	0.005%
56	8.763	2397	2402	2404	rBV	446	304	0.03%	0.003%
57	8.776	2404	2406	2410	rBV2	607	422	0.04%	0.005%
58	8.853	2419	2430	2460	rBV	484750	803122	76.39%	8.783%
59	9.358	2585	2587	2591	rVB2	270	166	0.02%	0.002%
60	9.506	2630	2633	2636	rBV	327	218	0.02%	0.002%
61	9.574	2650	2654	2655	rBV2	445	213	0.02%	0.002%
62	9.638	2671	2674	2677	rBV2	224	194	0.02%	0.002%
63	9.731	2700	2703	2707	rVB2	498	320	0.03%	0.003%
64	9.850	2737	2740	2743	rBV2	301	242	0.02%	0.003%
65	9.937	2763	2767	2768	rBV	324	191	0.02%	0.002%
66	10.130	2822	2827	2836	rVB7	1982	2567	0.24%	0.028%
67	10.217	2843	2854	2875	rBV	324173	513884	48.88%	5.620%
68	10.464	2927	2931	2934	rBV2	389	238	0.02%	0.003%
69	10.561	2959	2961	2964	rBV2	333	236	0.02%	0.003%
70	10.660	2989	2992	2996	rVB2	451	259	0.02%	0.003%
71	10.693	3000	3002	3005	rBV2	302	170	0.02%	0.002%
72	10.767	3019	3025	3027	rBV2	333	349	0.03%	0.004%
73	10.779	3027	3029	3034	rVB3	362	271	0.03%	0.003%
74	10.815	3038	3040	3043	rVB2	391	171	0.02%	0.002%
75	10.837	3043	3047	3049	rBV2	480	320	0.03%	0.003%
76	10.924	3067	3074	3080	rVB4	1742	2293	0.22%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022194.D
 Acq On : 17 Sep 2021 18:41
 Operator : SY/MD
 Sample : M3676-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.966	3082	3087	3088	rBV2	425	286	0.03%	0.003%
78	11.027	3101	3106	3108	rBV2	413	359	0.03%	0.004%
79	11.136	3138	3140	3143	rBV2	548	413	0.04%	0.005%
80	11.181	3151	3154	3157	rBV	251	176	0.02%	0.002%
81	11.252	3164	3176	3200	rBV	455662	711540	67.67%	7.782%
82	11.490	3247	3250	3253	rBV	345	246	0.02%	0.003%
83	11.541	3262	3266	3267	rBV2	370	218	0.02%	0.002%
84	11.567	3272	3274	3276	rVB	365	165	0.02%	0.002%
85	11.625	3280	3292	3314	rBV	450681	729072	69.34%	7.974%
86	11.911	3377	3381	3384	rBV2	313	259	0.02%	0.003%
87	12.017	3412	3414	3416	rBV2	337	187	0.02%	0.002%
88	12.194	3465	3469	3473	rBV3	268	263	0.03%	0.003%
89	12.410	3533	3536	3539	rBV2	416	270	0.03%	0.003%
90	12.583	3586	3590	3592	rBV2	299	206	0.02%	0.002%
91	12.606	3595	3597	3600	rVB	422	230	0.02%	0.003%
92	12.648	3608	3610	3613	rBV2	289	164	0.02%	0.002%
93	12.731	3631	3636	3640	rBV3	313	409	0.04%	0.004%
94	12.914	3691	3693	3699	rBV3	415	553	0.05%	0.006%
95	13.172	3770	3773	3775	rBV	391	218	0.02%	0.002%
96	13.416	3845	3849	3854	rBV2	272	231	0.02%	0.003%
97	13.509	3876	3878	3880	rBV2	357	237	0.02%	0.003%
98	13.622	3910	3913	3918	rBV	269	186	0.02%	0.002%
99	13.866	3985	3989	3993	rBV2	394	280	0.03%	0.003%
100	14.506	4186	4188	4196	rVB2	437	281	0.03%	0.003%


Sum of corrected areas: 9143569

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022194.D
Acq On : 17 Sep 2021 18:41
Operator : SY/MD
Sample : M3676-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0CE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

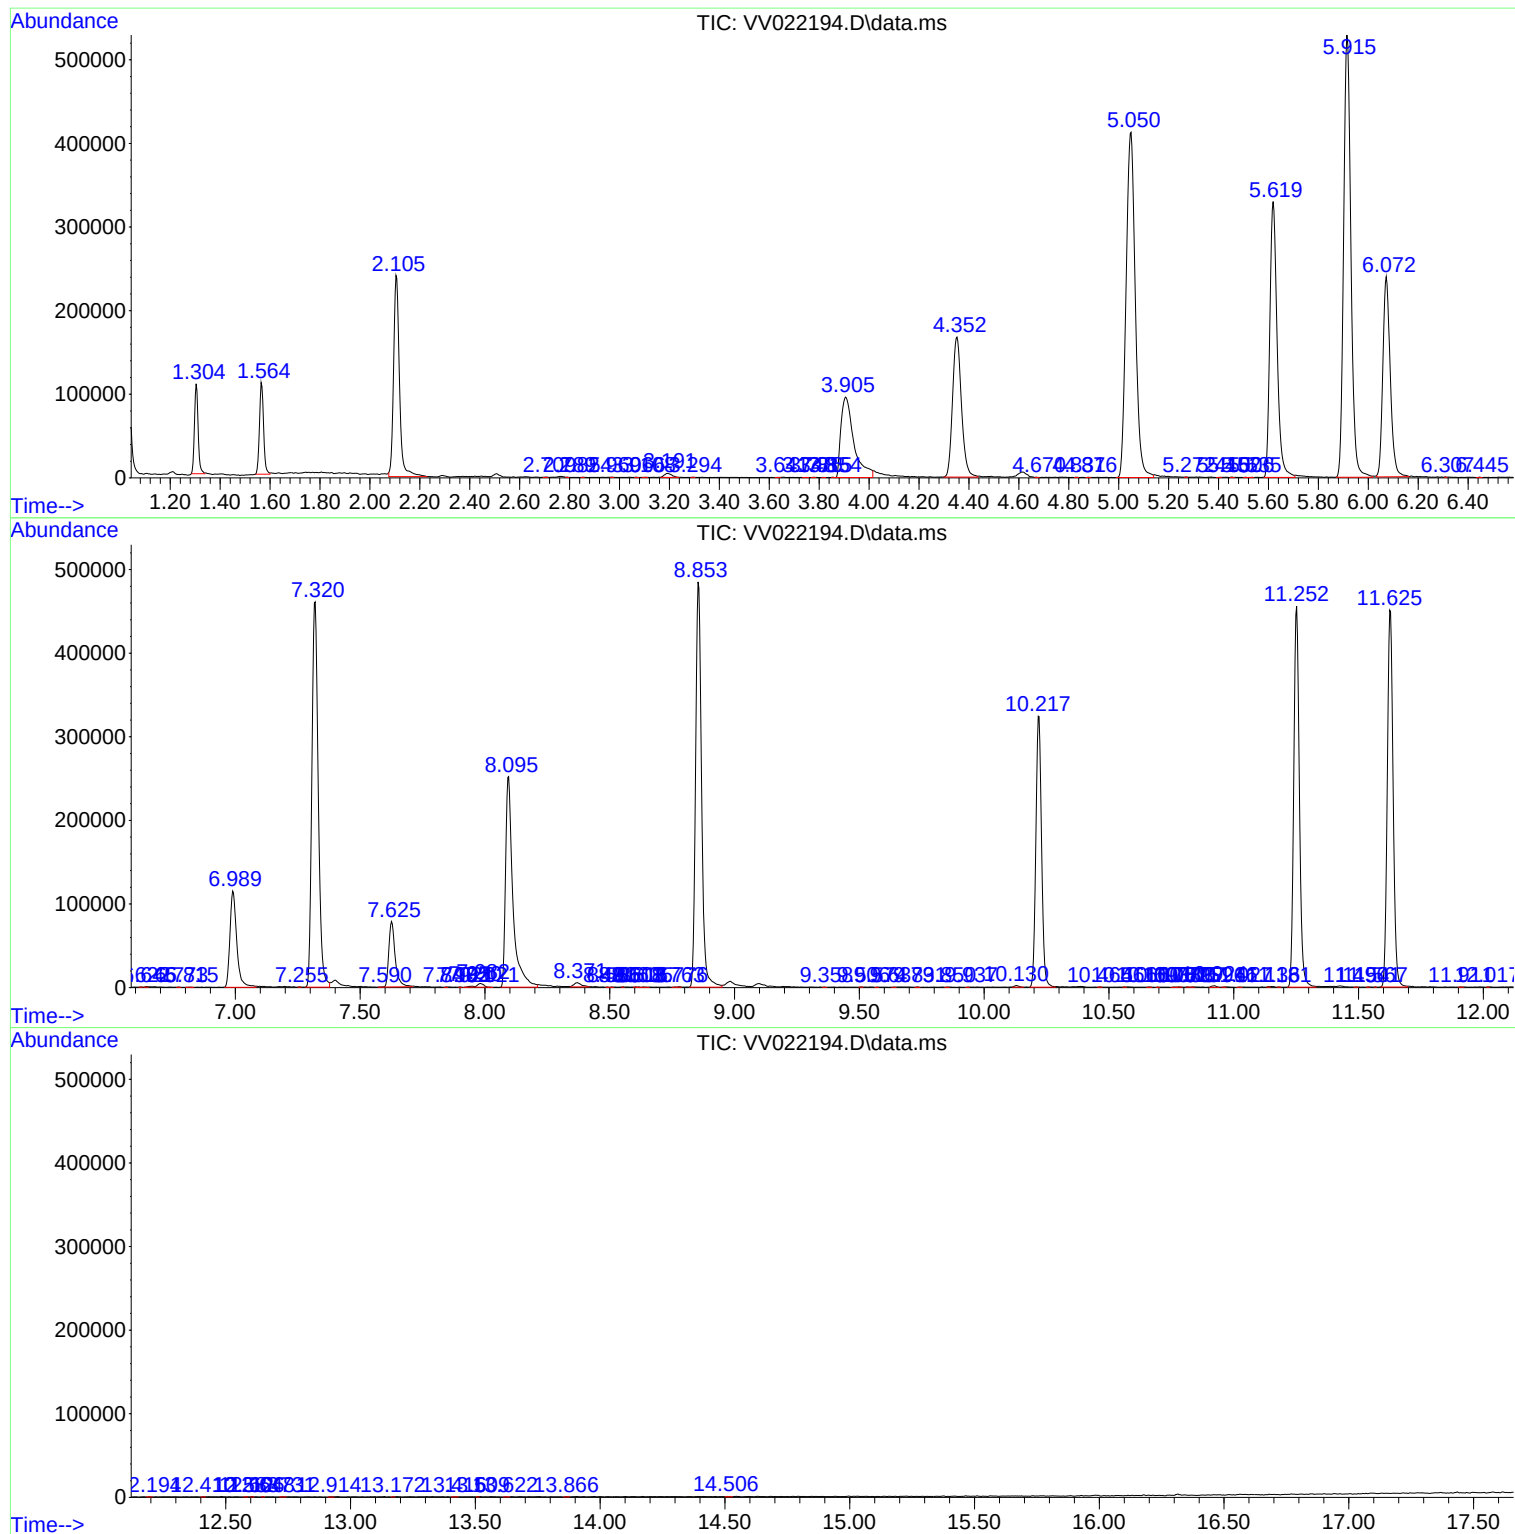

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022194.D
Acq On : 17 Sep 2021 18:41
Operator : SY/MD
Sample : M3676-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022194.D
Acq On : 17 Sep 2021 18:41
Operator : SY/MD
Sample : M3676-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
