

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022198.D
 Acq On : 17 Sep 2021 20:41
 Operator : SY/MD
 Sample : M3676-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022198.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	109259	115258	10.90%	1.390%
2	1.564	156	163	178	rBV	111537	125739	11.90%	1.516%
3	2.105	321	331	344	rBV	224976	326042	30.85%	3.932%
4	2.725	522	524	527	rVB3	761	312	0.03%	0.004%
5	2.764	532	536	540	rBV4	467	462	0.04%	0.006%
6	2.905	578	580	584	rVB3	404	237	0.02%	0.003%
7	3.015	610	614	618	rBV	212	253	0.02%	0.003%
8	3.117	643	646	653	rVB3	334	340	0.03%	0.004%
9	3.182	662	666	667	rBV2	278	173	0.02%	0.002%
10	3.207	671	674	678	rVB3	345	266	0.03%	0.003%
11	3.230	678	681	687	rBV2	231	245	0.02%	0.003%
12	3.330	706	712	714	rBV2	282	253	0.02%	0.003%
13	3.461	747	753	758	rBV2	335	229	0.02%	0.003%
14	3.513	765	769	776	rBV3	421	393	0.04%	0.005%
15	3.670	813	818	821	rBV2	256	231	0.02%	0.003%
16	3.693	821	825	826	rVV	221	155	0.01%	0.002%
17	3.777	847	851	854	rVB3	259	213	0.02%	0.003%
18	3.857	874	876	878	rBV	304	185	0.02%	0.002%
19	3.902	878	890	945	rVV2	86507	340909	32.25%	4.111%
20	4.352	1014	1030	1056	rBV	168704	418024	39.55%	5.041%
21	4.690	1133	1135	1139	rBV	418	287	0.03%	0.003%
22	4.764	1156	1158	1161	rBV	256	163	0.02%	0.002%
23	4.818	1173	1175	1178	rBV	264	149	0.01%	0.002%
24	4.838	1178	1181	1184	rVV	418	287	0.03%	0.003%
25	4.870	1188	1191	1194	rBV	335	223	0.02%	0.003%
26	4.947	1212	1215	1217	rBV2	285	199	0.02%	0.002%
27	5.047	1230	1246	1275	rBV2	417899	1057033	100.00%	12.747%
28	5.365	1342	1345	1347	rBV	299	193	0.02%	0.002%
29	5.416	1357	1361	1363	rVV	342	235	0.02%	0.003%
30	5.490	1381	1384	1385	rBV	366	189	0.02%	0.002%
31	5.558	1401	1405	1406	rBV	252	156	0.01%	0.002%
32	5.619	1412	1424	1454	rBV	339931	686211	64.92%	8.275%
33	5.834	1489	1491	1497	rVB4	501	277	0.03%	0.003%
34	5.860	1497	1499	1503	rVB	450	251	0.02%	0.003%
35	5.915	1503	1516	1540	rBV5	90883	201708	19.08%	2.432%
36	6.072	1552	1565	1587	rBV	243416	487102	46.08%	5.874%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V091721\
 Data File : V022198.D
 Acq On : 17 Sep 2021 20:41
 Operator : SY/MD
 Sample : M3676-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.297	1633	1635	1639	rBV	287	243	0.02%	0.003%
38	6.320	1639	1642	1650	rVB5	580	708	0.07%	0.009%
39	6.516	1699	1703	1706	rVB3	263	190	0.02%	0.002%
40	6.551	1706	1714	1718	rBV3	483	616	0.06%	0.007%
41	6.754	1774	1777	1781	rVB2	492	273	0.03%	0.003%
42	6.838	1800	1803	1805	rVV	283	158	0.01%	0.002%
43	6.911	1822	1826	1829	rBV3	257	224	0.02%	0.003%
44	6.989	1840	1850	1870	rBV	117054	213935	20.24%	2.580%
45	7.265	1934	1936	1938	rVB	510	198	0.02%	0.002%
46	7.317	1941	1952	1970	rBV	474844	824932	78.04%	9.948%
47	7.583	2031	2035	2037	rBV2	449	248	0.02%	0.003%
48	7.625	2038	2048	2065	rBV	79392	138306	13.08%	1.668%
49	7.802	2100	2103	2108	rVB3	598	530	0.05%	0.006%
50	7.841	2111	2115	2117	rBV3	328	175	0.02%	0.002%
51	7.982	2152	2159	2166	rBV7	3294	5218	0.49%	0.063%
52	8.095	2183	2194	2232	rBV2	272897	554097	52.42%	6.682%
53	8.516	2323	2325	2328	rVV3	410	287	0.03%	0.003%
54	8.548	2332	2335	2336	rBV3	363	201	0.02%	0.002%
55	8.571	2340	2342	2345	rBV2	334	170	0.02%	0.002%
56	8.616	2354	2356	2360	rVB2	316	175	0.02%	0.002%
57	8.654	2366	2368	2371	rBV3	508	213	0.02%	0.003%
58	8.751	2394	2398	2401	rBV4	512	459	0.04%	0.006%
59	8.789	2406	2410	2411	rBV	305	202	0.02%	0.002%
60	8.854	2419	2430	2455	rBV	497568	818718	77.45%	9.873%
61	9.108	2506	2509	2512	rBV3	294	199	0.02%	0.002%
62	9.140	2515	2519	2520	rBV2	519	360	0.03%	0.004%
63	9.204	2537	2539	2543	rVB	363	235	0.02%	0.003%
64	9.288	2560	2565	2568	rBV2	446	336	0.03%	0.004%
65	9.400	2597	2600	2603	rBV2	233	173	0.02%	0.002%
66	9.513	2631	2635	2638	rBV2	311	223	0.02%	0.003%
67	9.561	2644	2650	2655	rBV3	712	862	0.08%	0.010%
68	9.837	2731	2736	2739	rBV2	334	293	0.03%	0.004%
69	9.921	2759	2762	2764	rBV2	334	234	0.02%	0.003%
70	10.014	2789	2791	2794	rBV2	250	166	0.02%	0.002%
71	10.130	2820	2827	2832	rBV5	1633	2197	0.21%	0.026%
72	10.220	2843	2855	2875	rBV	322218	506291	47.90%	6.105%
73	10.461	2926	2930	2933	rVB3	622	467	0.04%	0.006%
74	10.542	2949	2955	2958	rBV3	417	468	0.04%	0.006%
75	10.661	2987	2992	2995	rBV3	423	472	0.04%	0.006%
76	10.680	2995	2998	3000	rBV	388	215	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022198.D
 Acq On : 17 Sep 2021 20:41
 Operator : SY/MD
 Sample : M3676-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.696	3000	3003	3007	rVB2	295	215	0.02%	0.003%
78	10.789	3028	3032	3036	rBV2	397	296	0.03%	0.004%
79	10.918	3066	3072	3074	rBV3	1791	1634	0.15%	0.020%
80	11.017	3101	3103	3108	rBV2	227	186	0.02%	0.002%
81	11.040	3108	3110	3113	rVB3	574	295	0.03%	0.004%
82	11.079	3118	3122	3123	rBV2	399	264	0.02%	0.003%
83	11.146	3138	3143	3144	rBV2	666	516	0.05%	0.006%
84	11.188	3153	3156	3158	rBV2	448	286	0.03%	0.003%
85	11.252	3165	3176	3202	rBV	466128	718498	67.97%	8.664%
86	11.513	3253	3257	3259	rBV2	221	164	0.02%	0.002%
87	11.535	3262	3264	3267	rBV2	549	376	0.04%	0.005%
88	11.625	3281	3292	3312	rVV	459099	728183	68.89%	8.781%
89	11.786	3340	3342	3348	rVB3	474	407	0.04%	0.005%
90	11.921	3381	3384	3387	rBV	550	306	0.03%	0.004%
91	12.046	3420	3423	3426	rBV2	245	190	0.02%	0.002%
92	12.169	3459	3461	3465	rBV2	473	278	0.03%	0.003%
93	12.223	3474	3478	3480	rBV2	436	244	0.02%	0.003%
94	12.361	3518	3521	3524	rBV	389	301	0.03%	0.004%
95	12.458	3548	3551	3555	rVB3	391	287	0.03%	0.003%
96	12.657	3610	3613	3618	rBV2	462	389	0.04%	0.005%
97	12.734	3633	3637	3638	rBV	287	194	0.02%	0.002%
98	13.750	3950	3953	3954	rBV2	581	326	0.03%	0.004%
99	13.934	4007	4010	4015	rBV3	390	285	0.03%	0.003%
100	14.017	4034	4036	4039	rBV	274	165	0.02%	0.002%




Sum of corrected areas: 8292534

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022198.D
Acq On : 17 Sep 2021 20:41
Operator : SY/MD
Sample : M3676-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

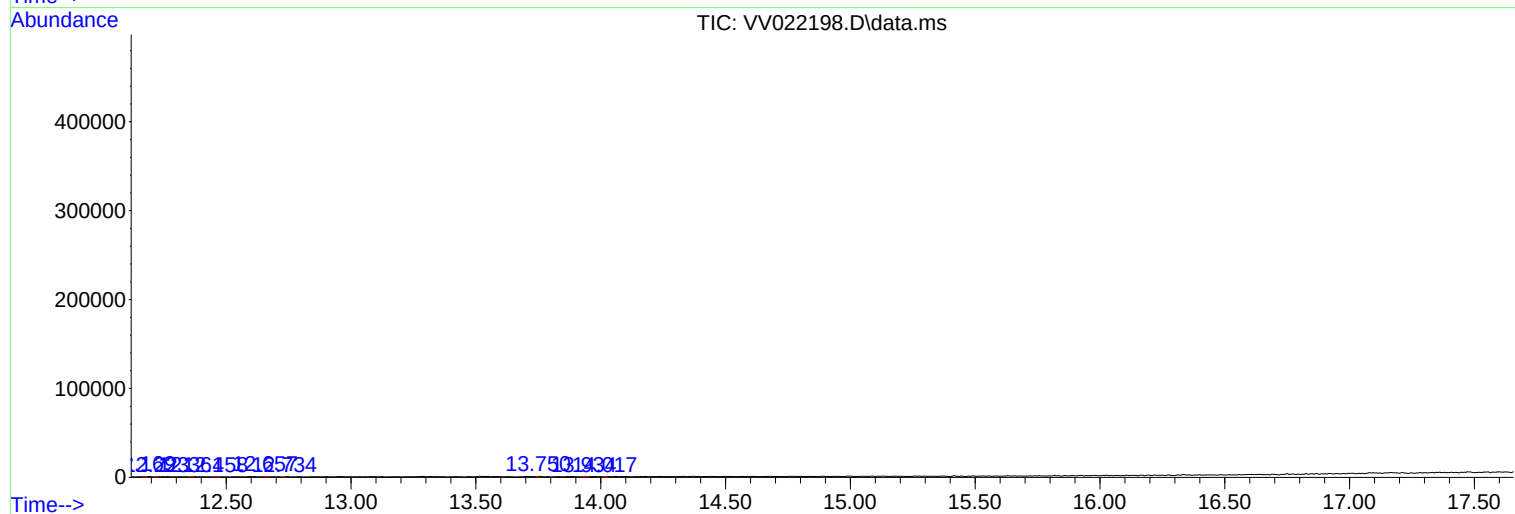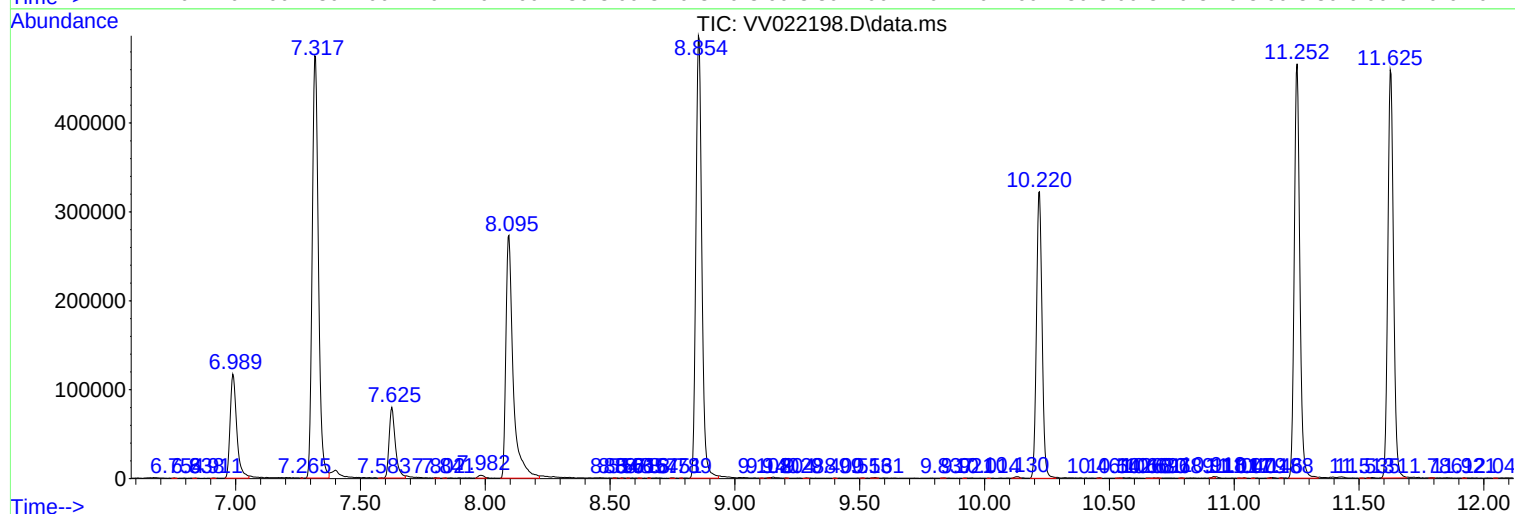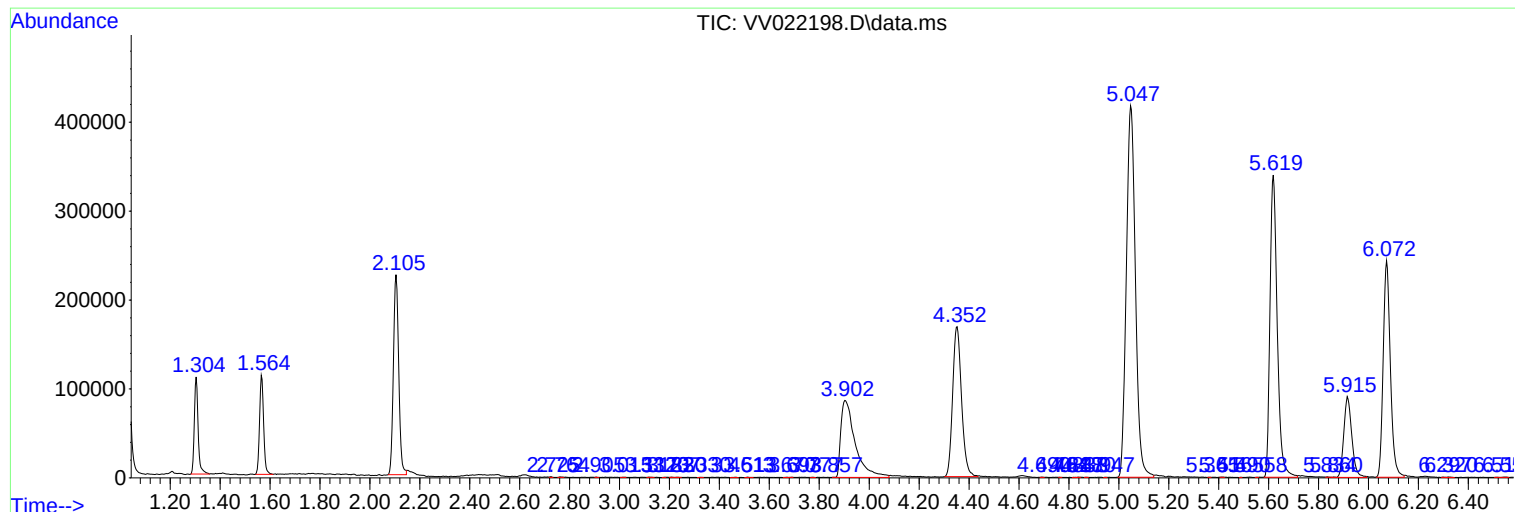

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022198.D
Acq On : 17 Sep 2021 20:41
Operator : SY/MD
Sample : M3676-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022198.D
Acq On : 17 Sep 2021 20:41
Operator : SY/MD
Sample : M3676-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
