

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022200.D
 Acq On : 17 Sep 2021 21:30
 Operator : SY/MD
 Sample : M3676-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022200.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	103	rVB	106307	112926	10.89%	1.376%
2	1.568	156	164	178	rBV	105020	120791	11.65%	1.472%
3	2.105	322	331	343	rBV	225676	322912	31.14%	3.936%
4	2.285	385	387	393	rBV4	725	645	0.06%	0.008%
5	2.780	536	541	544	rVB3	385	354	0.03%	0.004%
6	2.799	544	547	549	rBV2	272	156	0.02%	0.002%
7	2.886	572	574	577	rVB2	286	151	0.01%	0.002%
8	2.950	592	594	596	rBV	365	156	0.02%	0.002%
9	3.140	647	653	654	rBV	293	222	0.02%	0.003%
10	3.178	660	665	668	rBV3	352	400	0.04%	0.005%
11	3.224	676	679	681	rBV	375	218	0.02%	0.003%
12	3.378	724	727	729	rBV	291	138	0.01%	0.002%
13	3.445	744	748	751	rBV2	282	261	0.03%	0.003%
14	3.487	757	761	763	rBV2	227	153	0.01%	0.002%
15	3.535	773	776	778	rBV2	417	243	0.02%	0.003%
16	3.638	804	808	810	rVB	442	193	0.02%	0.002%
17	3.674	817	819	824	rVB2	322	199	0.02%	0.002%
18	3.905	880	891	948	rBV2	74455	297796	28.72%	3.630%
19	4.352	1013	1030	1058	rBV	166413	417518	40.26%	5.089%
20	4.603	1103	1108	1110	rBV4	1563	1449	0.14%	0.018%
21	4.709	1139	1141	1143	rBV2	293	150	0.01%	0.002%
22	4.805	1168	1171	1175	rBV3	343	317	0.03%	0.004%
23	4.863	1185	1189	1191	rBV3	377	340	0.03%	0.004%
24	4.969	1219	1222	1225	rBV2	194	159	0.02%	0.002%
25	4.992	1225	1229	1230	rBV2	331	205	0.02%	0.002%
26	5.050	1230	1247	1275	rBV2	407339	1037072	100.00%	12.640%
27	5.368	1342	1346	1348	rBV	316	267	0.03%	0.003%
28	5.500	1384	1387	1388	rBV2	298	185	0.02%	0.002%
29	5.535	1396	1398	1403	rVB2	563	381	0.04%	0.005%
30	5.561	1403	1406	1408	rVB2	242	153	0.01%	0.002%
31	5.619	1408	1424	1454	rBV	327122	669869	64.59%	8.165%
32	5.857	1496	1498	1501	rBV2	361	157	0.02%	0.002%
33	5.915	1501	1516	1541	rBV3	137971	293141	28.27%	3.573%
34	6.072	1552	1565	1587	rBV	233958	477288	46.02%	5.817%
35	6.378	1658	1660	1662	rVB	288	145	0.01%	0.002%
36	6.394	1662	1665	1666	rBV	287	146	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V091721\
 Data File : VV022200.D
 Acq On : 17 Sep 2021 21:30
 Operator : SY/MD
 Sample : M3676-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.439	1676	1679	1682	rBV	428	248	0.02%	0.003%
38	6.481	1690	1692	1698	rVV2	352	215	0.02%	0.003%
39	6.526	1702	1706	1710	rBV	445	295	0.03%	0.004%
40	6.548	1711	1713	1716	rVB2	355	147	0.01%	0.002%
41	6.731	1767	1770	1772	rVV2	293	170	0.02%	0.002%
42	6.760	1776	1779	1781	rBV	403	246	0.02%	0.003%
43	6.789	1786	1788	1791	rBV	267	192	0.02%	0.002%
44	6.863	1809	1811	1814	rBV2	372	175	0.02%	0.002%
45	6.886	1816	1818	1825	rVB2	267	249	0.02%	0.003%
46	6.921	1827	1829	1834	rVB2	286	171	0.02%	0.002%
47	6.944	1834	1836	1840	rBV3	507	351	0.03%	0.004%
48	6.989	1840	1850	1872	rBV	114339	209621	20.21%	2.555%
49	7.317	1939	1952	1972	rBV	475801	826030	79.65%	10.068%
50	7.625	2038	2048	2063	rBV	76040	134277	12.95%	1.637%
51	7.831	2110	2112	2114	rVB3	740	326	0.03%	0.004%
52	7.847	2114	2117	2118	rBV2	311	184	0.02%	0.002%
53	7.982	2154	2159	2171	rVB6	2478	3657	0.35%	0.045%
54	8.050	2178	2180	2182	rVB2	459	170	0.02%	0.002%
55	8.095	2182	2194	2231	rBV2	263170	539432	52.01%	6.575%
56	8.500	2318	2320	2324	rBV2	341	154	0.01%	0.002%
57	8.609	2351	2354	2356	rBV	321	170	0.02%	0.002%
58	8.625	2356	2359	2362	rVV2	357	207	0.02%	0.003%
59	8.654	2362	2368	2372	rVB2	376	434	0.04%	0.005%
60	8.680	2372	2376	2378	rBV2	312	208	0.02%	0.003%
61	8.812	2414	2417	2419	rBV	295	153	0.01%	0.002%
62	8.854	2419	2430	2455	rBV	490679	797219	76.87%	9.717%
63	9.127	2511	2515	2516	rBV2	436	268	0.03%	0.003%
64	9.185	2529	2533	2535	rBV	180	148	0.01%	0.002%
65	9.198	2535	2537	2541	rVB2	324	201	0.02%	0.002%
66	9.236	2545	2549	2551	rBV2	430	312	0.03%	0.004%
67	9.362	2586	2588	2591	rBV	342	218	0.02%	0.003%
68	9.390	2594	2597	2600	rVV2	337	159	0.02%	0.002%
69	9.497	2628	2630	2634	rVB3	256	144	0.01%	0.002%
70	9.599	2659	2662	2665	rBV	276	197	0.02%	0.002%
71	9.625	2667	2670	2673	rVV2	225	147	0.01%	0.002%
72	9.654	2675	2679	2682	rBV3	338	265	0.03%	0.003%
73	9.709	2692	2696	2702	rBV2	326	308	0.03%	0.004%
74	9.799	2720	2724	2726	rBV2	348	209	0.02%	0.003%
75	9.841	2735	2737	2739	rBV2	223	142	0.01%	0.002%
76	9.889	2748	2752	2754	rBV	219	167	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
 Data File : VV022200.D
 Acq On : 17 Sep 2021 21:30
 Operator : SY/MD
 Sample : M3676-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	9.915	2758	2760	2763	rVB2	358	150	0.01%	0.002%
78	9.998	2783	2786	2788	rBV2	265	169	0.02%	0.002%
79	10.114	2819	2822	2823	rBV	599	372	0.04%	0.005%
80	10.220	2843	2855	2878	rBV	312942	495717	47.80%	6.042%
81	10.387	2901	2907	2910	rBV2	696	620	0.06%	0.008%
82	10.435	2918	2922	2925	rBV2	303	270	0.03%	0.003%
83	10.554	2953	2959	2961	rBV3	544	479	0.05%	0.006%
84	10.577	2962	2966	2972	rVV3	469	389	0.04%	0.005%
85	10.921	3067	3073	3082	rVB5	1568	2294	0.22%	0.028%
86	11.152	3140	3145	3151	rVB5	678	764	0.07%	0.009%
87	11.252	3165	3176	3198	rBV	450554	709055	68.37%	8.642%
88	11.500	3251	3253	3257	rVB2	398	211	0.02%	0.003%
89	11.625	3281	3292	3313	rBV	449625	716882	69.13%	8.738%
90	12.005	3407	3410	3417	rBV2	340	423	0.04%	0.005%
91	12.821	3662	3664	3667	rBV	255	164	0.02%	0.002%
92	12.857	3672	3675	3677	rBV2	367	213	0.02%	0.003%
93	12.905	3687	3690	3694	rBV	424	305	0.03%	0.004%
94	12.966	3707	3709	3713	rBV	319	155	0.01%	0.002%
95	13.027	3726	3728	3731	rBV	326	188	0.02%	0.002%
96	13.699	3936	3937	3941	rBV2	308	233	0.02%	0.003%
97	13.763	3955	3957	3959	rBV	465	223	0.02%	0.003%
98	13.779	3959	3962	3966	rVB	470	311	0.03%	0.004%
99	14.072	4050	4053	4057	rVB3	552	425	0.04%	0.005%
100	14.091	4057	4059	4061	rBV3	333	173	0.02%	0.002%




Sum of corrected areas: 8204627

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022200.D
Acq On : 17 Sep 2021 21:30
Operator : SY/MD
Sample : M3676-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

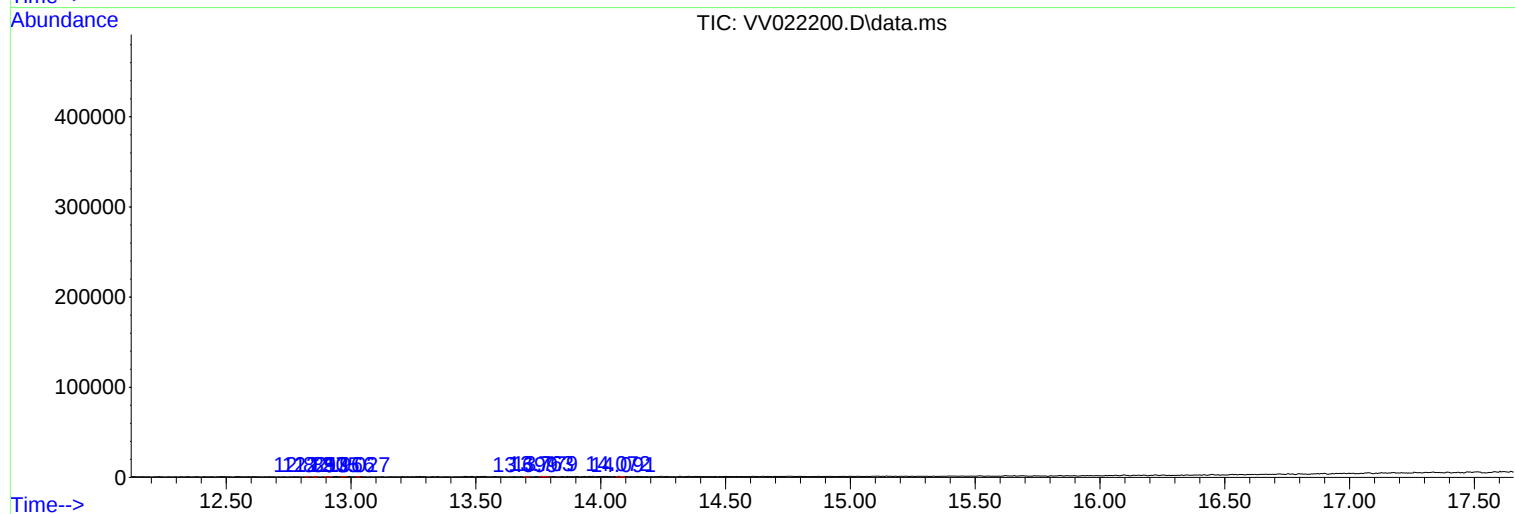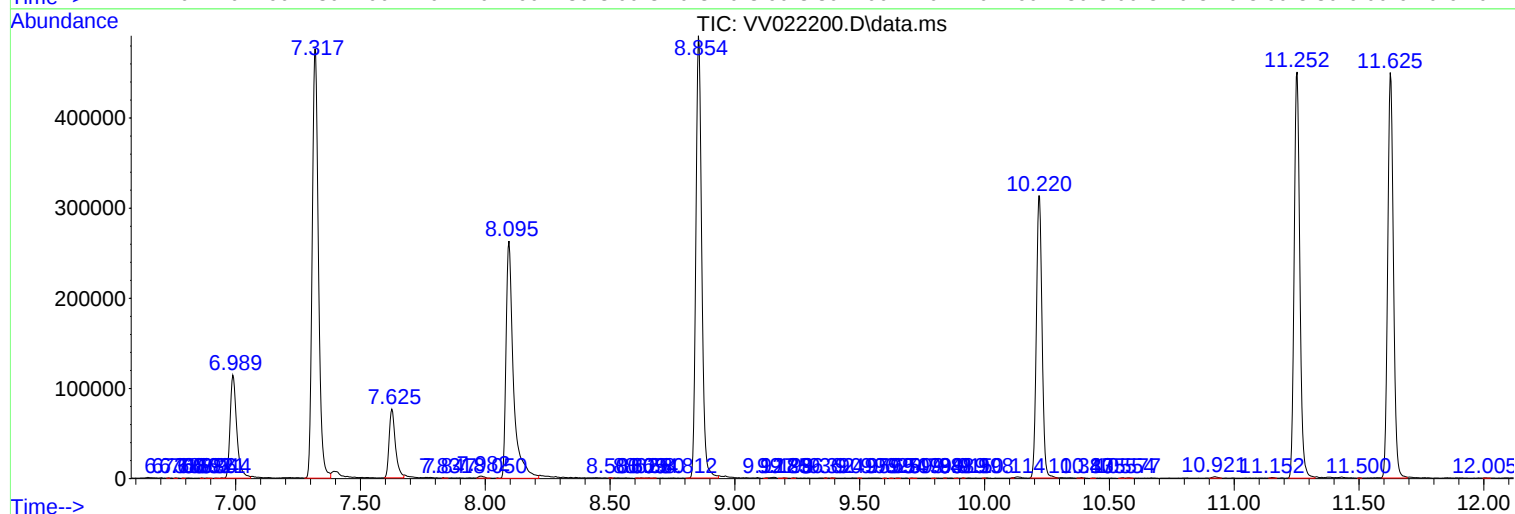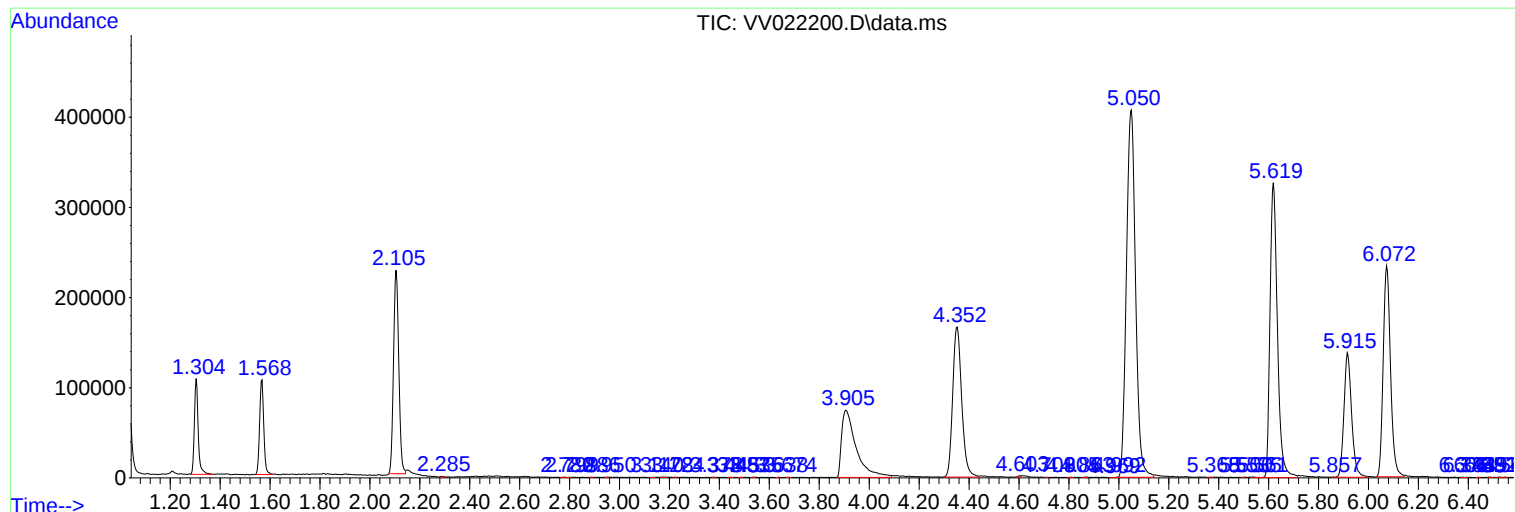

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022200.D
Acq On : 17 Sep 2021 21:30
Operator : SY/MD
Sample : M3676-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091721\
Data File : VV022200.D
Acq On : 17 Sep 2021 21:30
Operator : SY/MD
Sample : M3676-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
